

General Catalog





Metrohm – precision measurement systems for chemical analysis made in Switzerland

Metrohm AG, founded in 1943, is a worldwide leading manufacturer of precision instruments for chemical analysis. Our measurement instruments are found not only in the laboratories of practically every industry, but also in research institutes and government agencies.

At our headquarters in Herisau in eastern Switzerland, we develop and produce measurement instruments for titration, ion chromatography, pH and conductivity measurement, voltammetry and stability measurement. Our product program is supplemented with dosing and Liquid Handling systems, solutions for the automation of sample preparation and analysis and sensors, columns and extensive accessories. In addition, we have been distributing a newly introduced program of systems for near-infrared analyses in the laboratory and process under the brand name Metrohm NIRSystems since 2013.

Metrohm instruments are sold worldwide through a network of around 40 company-owned subsidiaries and through around 40 additional exclusive representatives. These also provide exclusive worldwide service and support under the name Metrohm.

We see ourselves as problem solvers – both in the laboratory and in the industrial process. It is for that reason that we offer our customers tailored overall solutions that, in addition to the respective analysis instruments, also comprise the necessary application expertise. At our applications laboratories, our chemists are continuously developing new applications and methods, publishing them in specialist journals and thereby opening up new fields of application for our customers.

Not at least, we distinguish ourselves from most of our – to some extent considerably larger – competitors by the fact that Metrohm AG has been wholly owned by the non-profit Metrohm Foundation since 1982.

Table of contents

pH/Conductivity measurement	1
Potentiometric and thermometric titration	11
Karl Fischer titration	33
Dosing devices	51
Automation in titration	59
Polarography, voltammetry and CVS	87
Stability measuring instruments	105
Near-infrared spectroscopy	113
Ion chromatography	129
Metrohm Quality Service	221



pH/Conductivity measurement






pH/Conductivity measurement

pH and Ion meters	4
pH meter overview	4
826 pH mobile	5
827 pH lab	6
780 pH Meter	7
781 pH/Ion Meter	8
867 pH Module	9
Conductometer	10
856 Conductivity Module	10

pH and Ion meters

pH meter overview

					
	826	827	780	781	867
Measuring range					
pH	0 ... 14 (-13 ... +20)		0 ... 14 (±20)		0 ... 14 (-13 ... +20)
mV	±1200		±2200		±1200
Temperature Pt 1000 [°C]	-150 ... +250		-150 ... +250		-150 ... +250
Temperature NTC [°C]	-5 ... +250		-20 ... +250		-5 ... +250
Concentration	-		- 10 ⁻³⁸ ... 10 ⁺³⁸		10 ⁻²¹ ... 10 ⁺²⁰
Resolution: pH	0.001		0.001		0.001
Resolution: U [mV]	0.1		0.1		0.1
Resolution: T [°C]	0.1		0.1		0.1
pH-calibration (number of buffers)	3		9		5 (Touch Control) / 9 (<i>tiamo</i> TM)
Stability control (drift display)	x		x		x
Plot function pH/mV/T versus time	-		x		x
Automatic buffer recognition	x		x		x
Saving of calibration data incl. graph	only data		graph and data		graph and data
Automatic temperature compensation	x		x		x
Automatic electrode test	-		x		with Touch Control / <i>tiamo</i> TM
Remote stirrer control	-		x		x
Handling of intelligent dosing elements	-		-		x
Automatic standard addition	-		- Dosimat		Dosino/Dosimat
Touch Control with color display or <i>tiamo</i> TM	-		-		x
Method memory	-		x		x
Result memory	x		x		x
Print out according to GLP/ISO	x		x		x
GLP/GMP and FDA compliance (21 CFR Part11)	-		-		Touch Control/ <i>tiamo</i> TM full
Additional input for intelligent electrodes	-		-		x
Ipol or Upol integrated polarizer	-		-		x
Printer connection	IrDA		RS232		USB
2 USB connections for sample processor, printer, ...	-		-		x
MSB connection	-		1 (stirrer)		4 (stirrer, Dosino)
Sample processor (optional)	-		remote		USB
Line operation with 100 ... 240 V, 50/60 Hz	Battery only		x		x
Lablink	-		-		x
Language	English		German, English, Spanish, French		German, English, Spanish, French, Chinese, Portuguese, Russian, Polish, Italian, Japanese; Touch Control additionally in Korean; <i>tiamo</i> TM additionally in Slovak and Traditional Chinese

826 pH mobile

The 826 pH mobile is a handy and very easy-to-operate pH meter with wireless Infrared interface for data transfer to a printer or PC. Numerous functions, e.g., input options for user and/or sample identification, three-point calibration with automatic buffer recognition and various monitoring functions make it possible to work in conformance with GLP anywhere. The measured value memory contains up to 200 measured values, including date, time and sample identification, and can be called up and/or sent to a printer or PC at any time. When the 6.0228.020 Primatrode is used, the 826 pH mobile fulfills protection class IP 67, i.e. even a brief immersion in water will not harm the instrument. Power supply is provided by means of four LR6, UM3 or AA batteries; approx. 750 hours operating time is possible in normal operations.



826 pH mobile

Ordering Information

2.826.0010	826 pH mobile
2.826.0020	826 pH mobile with Primatrode
2.826.0110	826 pH mobile with carrying case

827 pH lab

The 827 pH lab is a handy and very easy to operate pH meter with wireless Infrared interface for daily routine work in the laboratory. Numerous functions, e.g., input options for user and/or sample identification, three-point calibration with automatic buffer recognition, automatic measured value acceptance and various monitoring functions make working in conformance with GLP child's play. The measured value memory contains up to 200 measured values, including date, time and sample identification, and can be called up and/or sent to a printer or PC at any time.



827 pH lab

Ordering Information

2.827.0114	827 pH lab; 230 V, EU with Primatrode
2.827.0115	827 pH lab; 120 V, US with Primatrode
2.827.0117	827 pH lab; 240 V, AUS with Primatrode
2.827.0119	827 pH lab; 230 V, UK with Primatrode
2.827.0214	827 pH lab; 230 V, EU with Unitrode
2.827.0215	827 pH lab; 120 V, US with Unitrode
2.827.0217	827 pH lab; 240 V, AUS with Unitrode
2.827.0219	827 pH lab; 230 V, UK with Unitrode

780 pH Meter

Precision pH meter

The 780 pH Meter offers a multitude of opportunities for pH measurements that meet the highest standards. In addition to the general functions of pH, voltage and temperature measurement, the 780 pH Meter is equipped with an automatic stirrer control, a multi-point calibration with up to nine buffers, a method memory and various monitoring functions for calibration and servicing. The automatic electrode test in conformance with GLP permits objective assessment of the electrode and leaves nothing more to chance. Reliable and reproducible results are thus guaranteed. The large backlit multi-line display provides an overview and makes the individual settings easy. The bidirectional RS-232 interface enables data transfer to a printer or PC. A sample changer can be connected through the optional 6.2148.010 Remote Box.



780 pH Meter

Ordering Information

2.780.0010 780 pH Meter

781 pH/Ion Meter

Combined pH/ion meter

The 781 pH/Ion Meter offers a multitude of possibilities for pH and ion measurements that meet the highest standards. In addition to the general functions of pH, ion, voltage and temperature measurement, the 781 pH Meter is equipped with an automatic stirrer control, a multi-point calibration with up to 9 buffers (pH mode), a methods memory and various monitoring functions for calibration and servicing. The automatic electrode test for pH glass electrodes in conformance with GLP permits objective assessment of the electrode and leaves nothing more to chance. Reliable and reproducible results are thus guaranteed. The large backlit multi-line display provides an overview and makes the individual settings easy. The bidirectional RS-232 interface enables data transfer to a printer or PC. A sample changer can be connected through the optional 6.2148.010 Remote Box.

Three different modes are available for ion measurement: direct measurement, standard or sample addition. In the case of fully automated standard addition with an optional Dosimat, only the concentration of the standard and the desired quantity of addition steps need to be entered, the pH/ion meter takes care of the rest. Up to 19 standards can be used for the calibration for direct measurement.



781 pH/Ion Meter

Ordering Information

2.781.0010 781 pH/Ion Meter

867 pH Module

pH and ion measurement at the highest level is possible with the 867 pH Module. It can be used as stand-alone instrument in conjunction with a 900 Touch Control or as a supplement to a Titrand system.

In addition to measurements of pH, temperature, mV, I_{pol} , U_{pol} and concentration, standard additions (manual, dos, autos) can also be carried out. In addition to conventional sensors, intelligent electrodes – „iTrodes“ – can also be used for measurement with the 867 pH Module. A polarized measuring input is available in addition.

The 867 pH Module is a modern pH/ion meter with automatic stirrer control and the option of operating intelligent dosing elements.

The instrument is equipped with 2 USB interfaces for connecting USB printers, Autosamplers or barcode readers and 4 MSB interfaces for connecting stirrers or dosing devices of the 800 Dosino type (for the controlled adding of auxiliary solutions or for the automated feed-through of the standard addition).

Both in combination with the Touch Control as stand-alone pH meter and also integrated in **tiamo**TM full systems (from Version 2.0), it is in compliance with GLP and FDA requirements.



867 pH Module with 840 Touch Control

Ordering Information

2.867.0010	867 pH Module
2.867.0110	867 pH Module with Touch Control
2.867.0210	867 pH Module with tiamo TM light

Options

2.800.0010	800 Dosino
2.801.0010	801 Stirrer
2.802.0040	802 Stirrer (propeller stirrer) for 804 Ti Stand
2.804.0010	804 Ti Stand without stand rod
6.2151.000	Cable USB A – mini-DIN 8-pin

Conductometer

856 Conductivity Module

The 856 Conductivity Module can be used as stand-alone instrument in combination with a 900 Touch Control or as a supplement to a Titrand system.

The 856 Conductivity Module can perform measurements with the latest in conductivity measuring technology, the 5-ring conductivity measuring cells. They reach a very high linearity without platinization of the cells. This guarantees highest accuracy, and the cell constant, once determined, remains constant over a wide measuring range. In contrast to the 4-ring cells, the electrode can be immersed completely into the beaker. This means not only that beakers with different fill levels are no problem, but also that rapid mixing within the measuring cell can take place, even in stirred measuring solutions. Last but not least, the 5-ring conductivity measuring cell is very easy to clean, thanks to the removable cap.

With the help of the optional 6.2103.160 Adapter box, the classical Metrohm conductivity measuring cells can also continue to be used with the instrument.

Thanks to the galvanically separated measuring input, pH value and conductivity can be determined in the same beaker without interference in conjunction with the 867 pH Module.

The instrument is equipped with 2 USB interfaces for connecting USB printers, Autosamplers or barcode readers and 4 MSB interfaces for connecting stirrers or dosing devices of the 800 Dosino type (e.g., for adding auxiliary solutions).

Both in conjunction with the 900 Touch Control as stand-alone conductivity measurement instrument and as an integrated component in **tiamo**TM full (from Version 2.0), the 856 Conductivity Module is in compliance with GLP and FDA requirements.



856 Conductivity Module with **tiamo**TM

Ordering Information

2.856.0010	856 Conductivity Module
2.856.0110	856 Conductivity Module with Touch Control, including 5-ring conductivity measuring cell
2.856.0120	856 Conductivity Module with Touch Control, including conductivity measuring cell (stainless steel)
2.856.0210	856 Conductivity Module with tiamo TM light, including 5-ring conductivity measuring cell
2.856.0220	856 Conductivity Module with tiamo TM light, including conductivity measuring cell (stainless steel)

Options

2.801.0010	801 Stirrer
6.0915.100	5-ring conductivity measuring cell c = 0.7 cm ⁻¹ with Pt1000
6.0915.130	5-ring conductivity measuring cell c = 1.0 cm ⁻¹ with Pt1000
6.0916.040	Conductivity measuring cell made of stainless steel, c = 0.1 cm ⁻¹ , with Pt1000 (St.N)
6.2103.160	Adapter 4 x socket B – plug N
6.2151.000	Cable USB A – mini-DIN 8-pin



Potentiometric and thermometric titration



Potentiometric and thermometric titration

Potentiometric titrators – Overview	14	Potentiometric titrators – Titrino plus	26
		Titrino plus – Introduction	26
Potentiometric titrators – Titrande	15	Titrino plus	27
Titrande family	15	848 Titrino plus	27
Titrande	16	877 Titrino plus	27
888 Titrande with Touch Control	16	Titrino plus packages	28
888 Titrande with <i>tiamo</i> TM light	16	Food/Beverage Titrino plus	28
902 Titrande	16	Food/Beverage Titrino plus with printer	28
904 Titrande	16	Salt Titrino plus	28
904 Titrande	17	Salt Titrino plus with printer	28
905 Titrande	17	Oil Titrino plus	29
905 Titrande	17	Oil Titrino plus with printer	29
906 Titrande	17	Optional accessories	30
906 Titrande	18	USB Thermal printer Neo's	30
907 Titrande	18	801 Stirrer with stand	30
907 Titrande	18	802 Stirrer (propeller stirrer) for 804 Ti Stand	30
Titrande packages	19	804 Ti Stand without stand rod	30
Surf Titrande Ionic	19	804 Ti Stand with stand	31
Surf Titrande Two Phase	19	869 Compact Sample Changer	31
Surf Titrande NIO	19		
Plate Titrande	19	Thermometric titration	32
Oil Titrande	20	859 Titrotherm complete with <i>tiamo</i> TM	32
Food Titrande	20		
Pharm Titrande	20		
Input instruments and software	21		
900 Touch Control	21		
<i>tiamo</i> TM 2.4 Light CD: 1 license	21		
<i>tiamo</i> TM 2.4 Full CD: 1 license	21		
<i>tiamo</i> TM 2.4 Multi CD: 3 licenses	21		
Optional accessories	22		
800 Dosino	22		
800 Dosino	22		
801 Stirrer with stand	22		
802 Stirrer (propeller stirrer) for 804 Ti Stand	22		
804 Ti Stand without stand rod	23		
804 Ti Stand with stand	23		
805 Dosimat	23		
846 Dosing Interface	23		
856 Conductivity Module	24		
867 pH Module	24		
Potentiometric titrators – Ti-Touch	25		
916 Salt Ti-Touch	25		
916 Oil Ti-Touch	25		
916 Food Ti-Touch	25		

Potentiometric titrators – Overview



Potentiometric Titrators	Titrimo plus			Ti-Touch		Titrande								
	870	877	848	915	916	888	890	901	902	904	905	906	907	
Optional 2nd measuring interface	-	-	-	-	-	-	-	yes	yes	yes	yes	yes	yes	
Intelligent Sensor «ITrodes»	-	-	-	-	yes	yes	-	yes	yes	yes	yes	yes	yes	
Volumetric Karl Fischer Titration	yes	-	-	yes	-	-	yes	yes	-	-	-	yes	yes	
Ion Measurement / Standard addition	-	-	-	-	-	-	-	-	-	yes	yes	yes	yes	
pH Measurement	-	yes	yes	-	yes	yes	-	yes	yes	yes	yes	yes	yes	
Endpoint Titration	-	yes	yes	-	yes	yes	-	yes	yes	yes	yes	yes	yes	
Dynamic Equivalence Point Titration	-	-	yes	-	yes	yes	-	-	-	yes	yes	yes	yes	
Monotonic Equivalence Point Titration	-	yes	yes	-	yes	yes	-	-	-	yes	yes	yes	yes	
Liquid Handling	-	-	-	yes	-	-	-	yes	yes	yes	yes	yes	yes	
STAT Titration	-	-	-	-	-	-	-	-	yes	-	-	yes	yes	
Dosino Technology	-	-	-	yes	yes	-	-	yes	yes	-	yes	-	yes	
Software Control	-	-	-	-	-	yes	yes	yes	yes	yes	yes	yes	yes	
Touch Control	-	-	-	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	
Live Display	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	
Report Printing / LIMS	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	
PDF report without PC	-	-	-	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	
Balance Connection via RS232	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	yes	

Potentiometric titrators – Titrando

Titrando family

Depending on the model, the Titrando supports the titration modes DET (dynamic equivalence point titration), MET (monotonic equivalence point titration) and SET (titration to one or two specified endpoints), KFT (volumetric Karl Fischer titration) and pH-STAT.

Ion meter

Not only pH, voltage and temperature can be measured with the MEAS pH and MEAS CONC measuring modes. Direct concentration determination and standard addition with ion-selective electrodes are also possible.

Comprehensive Liquid Handling

Basic operations of everyday laboratory work such as pipetting, transferring, dosing, dispensing and diluting become child's play, thanks to the Liquid Handling functionality of the Titrando. Maximum accuracy and precision are guaranteed in the range of 10 µL to 100 mL.

Measuring input

The measuring interface of the Titrando is comprised of a connector for the intelligent „iTrodes“ electrodes, a high-ohm measuring input and a measuring input for polarizable electrodes, in addition to one separate reference input and one temperature input for Pt1000 or NTC temperature sensors. The resolution of the inputs is at 0.1 mV or 0.001 pH. Up to two galvanically isolated measuring interfaces can be installed.

MSB connector

Up to 4 Dosinos or Dosimats, 4 magnetic stirrers or rod stirrers and 4 Remote Boxes can be connected for automation with its four installed Metrohm Serial Buses (MSB connectors). This makes the modular Titrando system the most flexible titration system on the market. The „Plug-and-play“ functionality makes the manual configuration of peripheral devices superfluous; the Titrando recognizes the connected instrument automatically.

USB connector

Two USB ports are available for communication with balances, printers or other USB-capable instruments. Laboratory balances can be connected with the aid of an RS-232 converter.

The Dosino – space-saving modernity

With the Titrando, dosing is accomplished with Dosino and intelligent dosing unit, which are screwed directly onto the reagent bottle. All of the data about the reagent and the dosing unit required for the titration is stored in the integrated data chip. Each dosing unit is marked with a serial number and a cylinder number and is shipped with an individual certificate.

Intelligent electrodes „iTrodes“

The integrated memory chip enables the saving of important sensor data such as article and serial numbers, calibration data, calibration history, duration of use and calibration validity. All of the sensor data is uploaded automatically when a connection is made with the Titrando. This means that the possibility of mix-ups or editing errors is eliminated. The user is informed if the electrode type does not match the one defined in the method. Monitoring functions allow the exclusion of electrodes whose calibration data lies outside the limit values or whose calibration period has already expired.

Operation – The choice is up to you

The Touch Control is an ergonomic and up-to-date operating element with direct network connection. Thanks to the new „Favorites“, you now have direct access to the methods you use most frequently.

The titration software *tiamo*TM offers, in addition to the standard functions for controlling a Titrando via PC, numerous additional functionalities, e.g., a client/server database or true parallel titration.

Unlimited automation

Increasing numbers of samples, complicated sample preparation steps and unattended overnight operation soon justify the use of a sample changer. The Titrando is equipped with the necessary intelligence for controlling sample changers. Whether it be large or small sample capacity, one or two workstations, sample measuring, sample preparation, Liquid Handling, or rinsing and calibrating the electrodes – the USB Sample Processors offer a high degree of automation with low investment costs.

Titrando

888 Titrando with Touch Control (2.888.0110)

High-end titrator with built-in buret drive

- including 900 Touch Control, 801 Stirrer magnetic stirrer, exchange unit (20 mL) and combined „Ecotrode plus“ pH glass electrode
- dynamic (DET), monotonic (MET) and endpoint titration (SET)
- four MSB connectors
- **one galvanically isolated measuring interface** (also for intelligent „iTrodes“ electrodes)
- USB connector



888 Titrando with *tiamo*TM light (2.888.0210)

High-end titrator with built-in buret drive

- including titration software *tiamo*TM light, 801 Stirrer magnetic stirrer, exchange unit (20 mL) and combined „Ecotrode plus“ pH glass electrode
- dynamic (DET), monotonic (MET) and endpoint titration (SET)
- four MSB connectors
- **one galvanically isolated measuring interface** (also for intelligent „iTrodes“ electrodes)
- USB connector



902 Titrando (2.902.0010)

High-end titrator for use with intelligent electrodes – iTrodes – with

- up to four dosing systems of the 800 Dosino type
- Endpoint titration (SET)
- enzymatic and pH-STAT titrations (STAT)
- Dosing functions with monitoring (DOS), Liquid Handling
- four MSB connectors
- **one galvanically isolated measuring interface**
- USB connector



904 Titrando (2.904.0010)

High-end titrator for use with intelligent electrodes – iTrodes – with

- built-in buret drive
- dynamic (DET), monotonic (MET) and endpoint titration (SET)
- Measurement with ion-selective electrodes (MEAS CONC)
- Dosing functions with monitoring, Liquid Handling
- four MSB connectors
- **one galvanically isolated measuring interface**
- USB connector



904 Titrande (2.904.0020)

High-end titrator for use with intelligent electrodes – iTrodes – with

- built-in buret drive
- dynamic (DET), monotonic (MET) and endpoint titration (SET)
- Measurement with ion-selective electrodes
- Dosing functions with monitoring, Liquid Handling
- four MSB connectors
- **two galvanically isolated measuring interfaces**
- USB connector



905 Titrande (2.905.0010)

High-end titrator for use with intelligent electrodes – iTrodes – with

- up to four dosing systems of the 800 Dosino type
- dynamic (DET), monotonic (MET) and endpoint titration (SET)
- Measurement with ion-selective electrodes
- Dosing functions (DOS), Liquid Handling
- four MSB connectors
- **one galvanically isolated measuring interface**
- USB connector



905 Titrande (2.905.0020)

High-end titrator for use with intelligent electrodes – iTrodes – with

- up to four dosing systems of the 800 Dosino type
- dynamic (DET), monotonic (MET) and endpoint titration (SET)
- Measurement with ion-selective electrodes
- Dosing functions (DOS), Liquid Handling
- four MSB connectors
- **two galvanically isolated measuring interfaces**
- USB connector



906 Titrande (2.906.0010)

High-end titrator for use with intelligent electrodes – iTrodes – with

- built-in buret drive
- dynamic (DET), monotonic (MET) and endpoint titration (SET), enzymatic and pH-STAT titrations (STAT), Karl Fischer titration (KFT)
- Measurement with ion-selective electrodes
- Dosing functions with monitoring, Liquid Handling
- four MSB connectors and USB connector
- **one galvanically isolated measuring interface**



906 Titrand (2.906.0020)

High-end titrator for use with intelligent electrodes – iTrodes – with

- built-in buret drive
- dynamic (DET), monotonic (MET) and endpoint titration (SET), enzymatic and pH-STAT titrations (STAT), Karl Fischer titration (KFT)
- Measurement with ion-selective electrodes
- Dosing functions with monitoring, Liquid Handling
- four MSB connectors and USB connector
- **two galvanically isolated measuring interfaces**



907 Titrand (2.907.0010)

High-end titrator for use with intelligent electrodes – iTrodes – with

- up to four dosing systems of the 800 Dosino type
- dynamic (DET), monotonic (MET) and endpoint titration (SET), enzymatic and pH-STAT titrations (STAT), Karl Fischer titration (KFT)
- Measurement with ion-selective electrodes
- Dosing functions with monitoring, Liquid Handling
- four MSB connectors and USB connector
- **one galvanically isolated measuring interface**



907 Titrand (2.907.0020)

High-end titrator for use with intelligent electrodes – iTrodes – with

- up to four dosing systems of the 800 Dosino type
- dynamic (DET), monotonic (MET) and endpoint titration (SET), enzymatic and pH-STAT titrations (STAT), Karl Fischer titration (KFT)
- Measurement with ion-selective electrodes
- Dosing functions with monitoring, Liquid Handling
- four MSB connectors and USB connector
- **two galvanically isolated measuring interfaces**



Titrando packages

Surf Titrando Ionic (2.905.1010)

The Surf Titrando Ionic is based on the 905 Titrando and offers a complete package for the most common **analyses of ionic surfactants**. Apart from the titration software *tiamo*TM light and determination methods described in detail, you will also receive comprehensive accessories for your titrations.

Surf Titrando Two Phase (2.905.1020)

The Surf Titrando Two Phase is based on the 905 Titrando and offers a complete package for the most common **analyses of ionic surfactants**. Apart from the titration software *tiamo*TM light and determination methods described in detail, you will also receive comprehensive accessories for your titrations.

Surf Titrando NIO (2.905.2010)

The Surf Titrando NIO is based on the 905 Titrando and offers a complete package for the most common **analyses of non-ionic surfactants**. Apart from the titration software *tiamo*TM light and determination methods described in detail, you will also receive comprehensive accessories for your titrations.

Plate Titrando (2.905.2020)

The Plate Titrando is based on the 905 Titrando and offers a complete package for the most common **analyses of plating baths**. Apart from the titration software *tiamo*TM light and determination methods described in detail, you will also receive comprehensive accessories for your titrations.



Oil Titrando (2.905.3010)

The Oil Titrando is based on the 905 Titrando and offers a complete package for the most common analyses of **petrochemical** products. Apart from the titration software *tiamo*TM light and determination methods described in detail, you will also receive comprehensive accessories for your titrations.

Food Titrando (2.905.4010)

The Food Titrando is based on the 905 Titrando and offers a complete package for the most common **analyses of foodstuffs**. Apart from the titration software *tiamo*TM light and determination methods described in detail, you will also receive comprehensive accessories for your titrations.

Pharm Titrando (2.907.1020)


The Pharm Titrando is based on the 907 Titrando and offers a complete package for the most common **analyses of pharmaceutical products**. Apart from the titration software *tiamo*TM full and determination methods described in detail, you will also receive comprehensive accessories for your titrations.



Input instruments and software

900 Touch Control (2.900.0010)

Operating unit for the Titrandos, USB Sample Processors, 856 Conductivity Module, 867 pH Module and 846 Dosing Interface. Touch-sensitive, high-resolution color display, simple and intuitive operation, thanks to favorites for direct method access. With integrated Ethernet interface for direct connection to the Internet and USB interface for connecting USB printers or a USB memory stick.

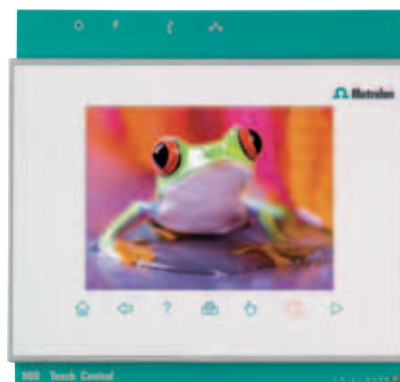

tiamo™ 2.4 Light CD: 1 license (6.6056.241)

Computer program for controlling a titration system.

- Up to two Metrohm instruments can be connected
- Graphical method editor with numerous templates
- Layout manager for individual monitor interface
- Database with reevaluation and report generator
- No parallel titration, no data export
- Languages: German, English, French, Italian, Spanish, Portuguese, Polish, Russian, Slovak, Japanese, Chinese, Traditional Chinese



tiamo™ 2.4 Full CD: 1 license (6.6056.242)

Computer program for controlling titration systems.

- Graphical method editor with numerous templates
- Layout manager for individual monitor interface
- Database with reevaluation and report generator
- Export to LIMS, NuGenesis, Cyberlab, etc.
- In compliance with the directives according to FDA 21 CFR Part 11
- Parallel titration
- Languages: German, English, French, Italian, Spanish, Portuguese, Polish, Russian, Slovak, Japanese, Chinese, Traditional Chinese



tiamo™ 2.4 Multi CD: 3 licenses (6.6056.243)

Computer program for controlling titration systems.

- Client/server version for network operation
- Graphical method editor with numerous templates
- Layout manager for individual monitor interface
- Database with reevaluation and report generator
- Export to LIMS, NuGenesis, Cyberlab, etc.
- In compliance with the directives according to FDA 21 CFR Part 11
- Parallel titration
- Languages: German, English, French, Italian, Spanish, Portuguese, Polish, Russian, Slovak, Japanese, Chinese, Traditional Chinese



Optional accessories

800 Dosino (2.800.0010)

Drive with write/read hardware for intelligent Dosing Units. With fixed cable (length 150 cm).



800 Dosino (2.800.0020)

Drive with write/read hardware for intelligent dosing units. With permanently attached cable (length 65 cm).



801 Stirrer with stand (2.801.0040)

Magnetic stirrer including base plate, support rod and electrode holder for supplementing the Titrino plus, Dosimat plus, Titrandos, Sample Processors, 805 Dosimat and 780/781 pH meters as well as the 856 and 867 measuring modules. With permanently attached cable for MSB (Metrohm Serial Bus).



802 Stirrer (propeller stirrer) for 804 Ti Stand (2.802.0040)

Rod stirrer with 6.1909.010 Propeller stirrer.



804 Ti Stand without stand rod (2.804.0010)

Titration stand and controller for 802 Stirrer. The 804 Ti Stand together with the optional 802 Stirrer provides an alternative to the magnetic stirrer. Without stand.



804 Ti Stand with stand (2.804.0040)

Titration stand and controller for 802 Rod Stirrer. The 804 Ti Stand together with the optional 802 Rod Stirrer provides an alternative to the magnetic stirrer. Ti Stand with base plate, support rod and electrode holder.



805 Dosimat (2.805.0010)

Dosing device for the Titrando and Sample Processors with read/write hardware for intelligent Exchange Units. With permanently attached cable. Without Exchange Unit.



846 Dosing Interface (2.846.0010)

USB-capable control unit for connecting a maximum of four 800 Dosinos or 805 Dosimats for dosing and Liquid Handling tasks. A Touch Control or the connection to a PC with *tiamo*[™], MagIC Net, viva or 797 VA Computrace is required for operation.



856 Conductivity Module (2.856.0010)

Conductivity measurement module as supplement to a Titrande or „stand-alone“ in combination with a 900 Touch Control.



867 pH Module (2.867.0010)

Module for pH/ion measurement as supplement to a Titrande or „stand-alone“ in combination with a 900 Touch Control.



Potentiometric titrators – Ti-Touch

916 Salt Ti-Touch (2.916.2010)

„Reduce to the max“ – this is the 916 Ti-Touch’s concept. The new compact Titrator from Metrohm offers the maximum in the class of stand-alone systems for routine analysis.

The „916 Salt Ti-Touch“ contains the complete accessories for chloride titration.

916 Oil Ti-Touch (2.916.3010)

„Reduce to the max“ – this is the 916 Ti-Touch’s concept. The new compact Titrator from Metrohm offers the maximum in the class of stand-alone systems for routine analysis.

The „916 Oil Ti-Touch“ contains the complete accessories for non-aqueous titration (acid number / base number).

916 Food Ti-Touch (2.916.4010)

„Reduce to the max“ – this is the 916 Ti-Touch’s concept. The new compact Titrator from Metrohm offers the maximum in the class of stand-alone systems for routine analysis.

The „916 Food Ti-Touch“ contains the complete accessories for the most important aqueous acid/base titrations – not only in the area of food analysis.



Potentiometric titrators – Titrino plus

Titrino plus – Introduction

The Titrino plus, Metrohm's entry class in the area of potentiometric titration, is particularly attractive due to its practically unbelievable price-performance ratio. A large live display with titration curve, „Plug & Play“ functionality of exchange unit, stirrer and USB printer, a high-precision measuring input, operation with keyboard – the Titrino plus offers considerably more than you would ever expect in this price segment. Their robustness also makes them the ideal titrators for routine determinations in everyday laboratory operations.

Potentiometric titration

The 877 Titrino plus supports the titration modes MET (monotonic equivalence point titration) and SET (titration to one or two specified endpoints). The 848 Titrino plus supports in addition the titration mode DET (dynamic equivalence point titration).

The live curve brings it to light

Every Titrino plus is equipped with a live curve display. This means that you are always informed of the progress of the titration.

Maximum precision thanks to the new measuring input

The Titrino plus is equipped with a high-resolution

measuring input that guarantees results with the greatest of precision.

Maximum ease of installation

The installation of a Titrino plus is designed to be exceptionally simple. Exchange unit, stirrer and USB compact printer are detected and configured automatically as soon as they are connected.

Mouse or keys – select your favorite!

The Titrino plus can be controlled either per mouseclick or keyboard. A USB port is available for communication with balances or printers. The optional 6.2148.030 USB/RS-232 adapter box enables the connection of laboratory balances and operation with a computer.

Intelligent exchange unit for more convenience

The chip for the intelligent Metrohm exchange unit automatically provides the titrator with the data (cylinder volume, type of reagent, date of expiration for the titer, etc.) that it requires to accomplish the titrations error-free. This means that you will always titer under optimum conditions and that you will not need, for example, to repeat any measurements because of an expired titer.



Titrimo plus

848 Titrimo plus (2.848.0010)

Compact titrator for

- dynamic (DET) titrations with automatic equivalence point finding
- monotonic (MET) titrations with automatic equivalence point finding
- endpoint titrations (SET)



877 Titrimo plus (2.877.0010)

Compact titrator for

- potentiometric endpoint titrations (SET)
- monotonic titrations with automatic equivalence point finding (MET)



Titrimo plus packages

Food/Beverage Titrimo plus (2.848.1010)

The Food/Beverage Titrimo plus offers you the complete package for all conventional analyses in food analysis. In addition to the more than 100 determination methods described in detail, you also receive the accessories for your titrations.

Food/Beverage Titrimo plus with printer (2.848.1020)

The Food/Beverage Titrimo plus offers you the complete package for all conventional analyses in food analysis. In addition to the more than 100 determination methods described in detail, you also receive the accessories for your titrations. Including USB thermal printer Neo's.



Salt Titrimo plus (2.848.2010)

The Salt Titrimo plus offers you the complete package for the analysis of chloride in a wide variety of samples. In addition to the determination methods described in detail, you also receive the complete accessories for your titrations.

Salt Titrimo plus with printer (2.848.2020)

The Salt Titrimo plus offers you the complete package for the analysis of chloride in a wide variety of samples. In addition to the determination methods described in detail, you also receive the complete accessories for your titrations. Including USB thermal printer Neo's.

Oil Titrino plus (2.848.3010)

The Oil Titrino plus offers you the complete package for the determination of the acid and base numbers of oil products. In addition to the determination methods described in detail, you also receive the complete accessories for your titrations.

Oil Titrino plus with printer (2.848.3020)

The Oil Titrino plus offers you the complete package for the determination of the acid and base numbers of oil products. In addition to the determination methods described in detail, you also receive the complete accessories for your titrations. Including USB thermal printer Neo's.



Optional accessories

USB Thermal printer Neo's (2.141.0100)

Compact printer with USB interface for the Titrino plus and Dosimat plus.

Paper width 60 mm (40 characters). Including 6.2151.120 USB cable.



801 Stirrer with stand (2.801.0040)

Magnetic stirrer including base plate, support rod and electrode holder for supplementing the Titrino plus, Dosimat plus, Titrandos, Sample Processors, 805 Dosimat and 780/781 pH meters as well as the 856 and 867 measuring modules. With permanently attached cable for MSB (Metrohm Serial Bus).



802 Stirrer (propeller stirrer) for 804 Ti Stand (2.802.0040)

Rod stirrer with 6.1909.010 Propeller stirrer.



804 Ti Stand without stand rod (2.804.0010)

Titration stand and controller for 802 Stirrer. The 804 Ti Stand together with the optional 802 Stirrer provides an alternative to the magnetic stirrer. Without stand.



804 Ti Stand with stand (2.804.0040)

Titration stand and controller for 802 Rod Stirrer. The 804 Ti Stand together with the optional 802 Rod Stirrer provides an alternative to the magnetic stirrer. Ti Stand with base plate, support rod and electrode holder.



869 Compact Sample Changer (2.869.0010)

The 869 Compact Sample Changer offers automation in a minimum amount of space.



Thermometric titration

859 Titrotherm complete with *tiamo*TM

Computer-controlled titrator for thermometric titration. Including complete accessories for the titration (10 mL buret, titration stand with rod stirrer, Thermoprobe, titration vessel and *tiamo*TM light).

Benefits of thermometric titration

- Rapid and robust method for routine operation
- One sensor for all applications – no interacting with the sample or the solvent
- Maintenance-free sensor – no calibration necessary
- Suitable for aggressive media
- No membrane or diaphragm problems

Thermometric titration is a highly versatile determination method. In principle, it is suitable for every reaction that causes a sufficiently large temperature change in the sample solution. It is therefore particularly suitable for applications

- for which no suitable potentiometric sensor or reference electrolyte is available
- for which the sample disrupts the electrode
- for which no solvent suitable for potentiometry is available



859 Titrotherm

The Titrotherm 859 – state-of-the-art USB technology

Thanks to state-of-the-art USB technology, the instrument is detected and configured automatically by the *tiamo*TM titration software at the time of connection to the computer. The same applies to all the dosing units, stirrers and sensors connected to the Titrotherm.

The proven *tiamo*TM software enables a rapid, goal-oriented method development, in addition to a simple generation of results. The endpoints are determined automatically; reproducibility can be enhanced even more when additional optimization parameters are used. The generation of reports is accomplished using method-specific form sheets that can be designed to suit.

Thermoprobe – rapid, precise and robust

The temperature sensor (thermistor) based on semiconductor technology has impressive properties: Its response time is only 0.3 s and its resolution is 10⁻⁵ K, thus enabling it to follow every temperature change both rapidly and precisely. The glass shaft lends the sensor an outstanding resistance to many organic solvents and aggressive media.

The Dosino technology

The Dosino technology from Metrohm has set a new standard in volumetric titration. The dosing unit is mounted together with the motor drive and the reagent bottle, thus guaranteeing maximum precision with minimum space requirements.

Catalyzed thermometric titration

In the event of very low sample concentrations or with low molar reaction enthalpy, the temperature change during the titration is often not sufficient for unambiguous determination of the endpoint, as for example with the determination of very small quantities of organic acids with the titrant $c(\text{KOH}) = 0.1 \text{ mol/L}$ in isopropanol. Here the addition of a small amount of paraformaldehyde facilitates the finding of the endpoint, because immediately after the endpoint is reached (i.e. as soon as excess hydroxide ions are present), the base-catalyzed hydrolysis of the paraformaldehyde starts. This strongly endothermic reaction now provides a sharp endpoint.

Ordering Information

2.859.1010 859 Titrotherm complete with *tiamo*TM



Karl Fischer titration



Karl Fischer titration

Introduction to Karl Fischer titration	36
Volumetric KF titrators	37
Volumetric KF titrators – Overview	37
890/901 Titrande	38
915 KF Ti-Touch	39
870 KF Titrino plus	40
KF Coulometer	41
Coulometric KF titrators – Overview	41
851/852 Titrande	42
756/831 KF Coulometer	43
899 Coulometer	44
Manual KF Sample Preparation	45
Polytron PT 1300 D	45
KF Evaporator	45
860 KF Thermoprep	45
Automated KF Sample Preparation	46
874 USB Oven Sample Processor	46
885 Compact Oven Sample Changer	47
KF Automation	48
Automated coulometric KF titrations	48
Automated volumetric KF titrations	48
Automated volumetric KF titration including sample preparation	48
KF Gas Analyzer	49
875 KF Gas Analyzer	49

Introduction to Karl Fischer titration

Karl Fischer water determination is one of the world's most frequently applied laboratory methods. In contrast to other water determinations, it is specific, rapid and requires very little apparatus.

With an application range of **0.1% to 100% water**, **volumetric Karl Fischer titration** is used in a wide variety of industries. Volumetry has the advantage that not only liquid but also solid and pasty samples can be added directly to the titration vessel. No matter whether you would like to determine water in foods, cosmetics or pharmaceutical products, you can never go wrong with the Metrohm KF titrators.

Coulometry is the optimum method for water determination in liquids, solids and gases for water contents in the trace range (**10 µg to 10 mg absolute water**). In addition, coulometry is an absolute method and thus no titer determination is required.





For difficult samples, we offer you intelligent solutions for **sample preparation**, e.g., the KF oven technique or sample pulverization with a homogenizer integrated in the system.

The use of automated systems pays off very quickly with high numbers of samples. Metrohm **KF Automation** offers you sophisticated techniques, not only for volumetric but also for coulometric KF titration.



Volumetric KF titrators

Volumetric KF titrators – Overview

				
Technical specifications	870 KF Titrino plus	915 Ti-Touch	890 Titrand	901 Titrand
Titration to preset pH/mV endpoints (SET)	–	–	–	yes
pH calibration and pH measurements (CAL, MEAS)	–	–	–	yes
Real-time curve display	yes	yes	yes	yes
Predefined methods	yes	yes	yes	yes
Parallel titration	–	–	–	yes (tiamo™)
Dosing drive for titration	Exchange Unit	Dosing Unit (optional Exchange Unit)	Exchange Unit	Dosing Unit (optional Exchange Unit)
Inputs, interfaces				
Second, galvanically separated measuring interface	–	–	–	option
Automated reagent exchange with Dosino (option)	–	yes	–	yes
MSB-port for connection of further Dosinos (addition of auxiliary solution, ...)	–	2	3	4
MSB-port for connection of further Dosinos (Titration)	–	2	–	4
Attachment of stirrer	yes	yes	yes	yes
Internal stirrer and pump	–	yes	–	–
Sample changer connection	–	yes	yes	yes
Attachment of printer, balance, ...	USB (1)	USB (1)	USB (2)	USB (2)
Optional interfaces	optional RS 232C	Ethernet (RJ-45)	optional RS 232C	optional RS 232C
Software				
tiamo™	–	–	yes	yes
tiBase™	yes	yes	yes	yes
Touch Control	–	integrated Touch Control	yes	yes

890/901 Titrandos

The KF titrators for the modern titration laboratory

Thanks to their **simple and intuitive operation** the KF Titrandos are the optimum instruments not only for **routine work** but also for **sophisticated applications in the development laboratory**. With the KF Titrandos, you have a titration system that can adapt to all imaginable requirements and demands no compromises.

An electrode test and the specially created „safety stop“ parameter prevent cell overflows during conditioning, i.e. conditioning is stopped after a given time or after a given volume of KF reagent has been added (**laboratory safety**). The sophisticated control algorithm of the Titrandos is tailored to the characteristics of the Karl Fischer reaction and guarantees maximum-precision results.

The choice is up to you! Both the 901 Titrandos and the 890 Titrandos can be optionally controlled either as stand-alone systems with Touch Control or through the PC with **tiamo™**.



901 Titrandos with 900 Touch Control

901 Titrandos

In addition to the Karl Fischer mode (KFT), the 901 Titrandos is also equipped with the SET mode and can thus perform titrations at a predefined endpoint. As a result of the high-resolution, galvanically isolated measuring interface with additional digital measuring input for the intelligent „iTrodes“ electrodes, it is additionally possible to perform pH measurements with a maximum of precision. Thanks to the four MSB connectors, up to four 800 Dosino dosing systems can be connected to the 901 Titrandos. These can be used not only for titration, but also for the automated addition of sample, standard and auxiliary solutions such as solubility promoters. Furthermore, all Liquid Handling commands are available. Thanks to its „Empty“ command, the Dosino may be completely emptied; this makes it possible to dispense with the tasks of opening and cleaning the dosing unit.

890 Titrandos

The 890 Titrandos offers the same high-end features as the 901 Titrandos (except for the digital measuring input), but is restricted to the KF mode and titrates exclusively with the proven exchange unit. In addition, up to three 800 Dosino dosing systems can be connected and used for the automatic addition of sample, standard and auxiliary solutions.

Ordering Information

2.890.0110	890 Titrandos with Touch Control
2.890.0210	890 Titrandos with tiamo™ light
2.901.0010	901 Titrandos

Options

2.800.0010	800 Dosino
2.803.0010	803 TI Stand with stirrer and pump
2.900.0010	900 Touch Control
6.2061.010	Bottle holder for Dosinos
6.3026.150	Exchange Unit 5 mL
6.3026.210	Exchange Unit 10 mL
6.3026.220	Exchange Unit 20 mL
6.3032.120	Dosing Unit 2 mL
6.3032.150	Dosing Unit 5 mL
6.3032.210	Dosing Unit 10 mL
6.3032.220	Dosing Unit 20 mL
6.6056.241	tiamo™ 2.4 Light CD: 1 license
6.6056.242	tiamo™ 2.4 Full CD: 1 license
6.6056.243	tiamo™ 2.4 Multi CD: 3 licenses

915 KF Ti-Touch

- Buret, stirrer, dosing unit, membrane pump and Touch Control in a single compact unit
- Contact-free reagent replacement
- Intranet and LIMS access – without PC
- Generating PDF reports – without a PC
- USB port for USB flash drive, printer, barcode reader, etc.
- One-touch titration

„Reduce to the max“ – that is the concept behind the 915 KF Ti-Touch. The new compact titrator for Karl Fischer titration from Metrohm offers the maximum in the class of stand-alone systems for routine analysis.

The sophisticated control algorithm of the 915 KF Ti-Touch is tailored to the characteristics of the Karl Fischer reaction and guarantees maximum-precision results. In addition, you can select a polarized alternating current (Ipol) or a defined voltage (Upol) to be applied to the electrode. Both working methods ensure fast, true results.



915 KF Ti-Touch

Different reagents require different parameters. The 915 KF Ti-Touch allows for the pertinent method to be selected for the different reagents.

Due to its simple and intuitive operation, it is the optimal instrument for routine work.

For example, the KF icons show you at a glance whether the instrument still needs to be conditioned or whether you can start the water determination. The electrode test and the „safety stop“ parameter prevent cell run-over during conditioning. If, for example, the electrode is not connected correctly or the titration cell is very humid, conditioning is stopped automatically after a given time or after a given volume of KF reagent has been added. This function increases work safety in your laboratory.

Automatic, contact-free reagent replacement

Replacing the used KF reagent in the titration cell may be carried out manually using the integrated membrane pump. Automated replacement is even more convenient. You determine the moment and the instrument performs the replacement automatically together with a Dosino. In both cases, contact with harmful reagents is avoided.

The Dosino – the optimum KF dosing system

Thanks to its „Empty“ command, the Dosino may be completely emptied; this makes it possible to eliminate the task of opening and cleaning the dosing unit, which is particularly annoying with KF reagents. Once the reagent is used up, the remaining content in the cylinder may be directly returned to the bottle or the titration vessel. Then the empty reagent bottle is replaced, the „preparing“ routine may be carried out via 915 KF Ti-Touch and the titer determination of the new reagent is ready to be started. In contrast to the exchange unit, repeated rinsing prior to titer determination is not necessary; this means you save on both time and reagents.

Ordering Information

2.915.0110 915 KF Ti-Touch

870 KF Titrino plus

- Maximum ease of installation
- Uncomplicated operation thanks to predefined methods and formulas
- Maximum precision thanks to high-resolution measuring input
- Live curve for detecting side reactions
- Overflow protection for enhanced work safety
- USB interface for compact printer

The inexpensive 870 Titrino plus is a KF titrator for volumetric water content determination. With it, water contents from a few ppm to 100% can be determined reliably and precisely in solid, liquid and gaseous samples. With its new user interface, which is tailored to routine users, the 870 Titrino plus is so simple to operate that only brief orientation periods are required. It is the ideal titrator for routine determinations, also because of its robustness. Titration vessel and electrode are included in the scope of delivery.



870 KF Titrino plus with 803 Ti Stand

Maximum ease of installation

The installation of the 870 Titrino plus is designed to be exceptionally simple. Exchange unit, stirrer and USB compact printer are detected and configured automatically as soon as they are connected.

Ready-to-use methods make work easier

You need only decide whether you wish to carry out a titer, blank value or water content determination and then start the titration with the single press of a key. Parameters need to be adjusted only in exceptional cases.

Mouse or keys – select your favorite!

The 870 Titrino plus is the first titrator that can be controlled either per mouseclick or keyboard.

Maximum precision

Just as is the case with the high-end Titrando titrator, the 870 KF Titrino plus is equipped with a high-resolution measuring input that guarantees results with the greatest of precision.

The live curve brings side reactions to light

Metrohm KF titrators are standard-equipped with a live curve display. Side reactions can thus be recognized and suppressed in time.

Great importance is placed on work safety in the handling of the harmful KF reagents. The overflow of iodine solution from the titration vessel is prevented by the „Conditioning options“ safety parameter.

Optional:

The 803 KF Titration Stand






The 803 KF Titration Stand is used for stirring and for the replacement of the exhausted working medium. With the integrated pump it is possible to aspirate the titrated solution and to add new solvent without opening the cell.

Ordering Information

2.870.0010	870 KF Titrino plus
2.870.1010	870 KF Titrino plus complete
2.870.1020	870 KF Titrino plus with printer
2.870.2010	870 KF Titrino plus and 860 KF Thermoprep

KF Coulometer

Coulometric KF titrators – Overview

					
Technical specifications	756 KF Coulometer	831 KF Coulometer	851 Titrand	852 Titrand	899 Coulometer
Coulometric Karl Fischer titration (KFC)	yes	yes	yes	yes	yes
Volumetric Karl Fischer titration (KFT)	–	–	–	yes	–
Bromine index (BRC)	–	–	yes	yes	–
Titration to preset mV endpoints (MET I_{pol} , SET U_{pol})	–	–	–	yes	–
Monotonic equivalence point titration (MET I_{pol} , MET U_{pol})	–	–	–	yes	–
Water/time real-time curve display	yes	yes	yes	yes	yes
Predefined methods	yes	yes	–	–	yes
Parallel titration	–	–	yes (with <i>tiamo</i> TM)	yes (with <i>tiamo</i> TM)	–
Automatic reagent exchange with Dosino (option)	yes	yes	yes	yes	–
Automatic titration start for coulometry	–	–	yes	yes	yes
Inputs, interfaces					
MSB-port for connection of further Dosinos (titration)	–	–	–	3	–
MSB-port for connection of further Dosinos (dosing)	–	–	yes	yes	–
Attachment of stirrer	yes	yes	yes	yes	yes
Sample changer connection	yes	yes	yes	yes	yes
Attachment of printer and balance	RS 232C	RS 232C	USB	USB	USB
Optional interfaces	RS 232C	RS 232C	RS 232C	RS 232C	RS 232C
Software					
<i>tiamo</i> TM	yes	yes	yes (2.1 or higher)	yes (2.1 or higher)	–
<i>tiBase</i> TM	–	–	yes	yes	yes
Touch Control	–	–	yes	yes	–

851/852 Titrande

Coulometry is the ideal method for water determination in liquids, solids and gases when it comes to water determination in the trace range (10 µg to 10 mg absolute water). In addition, coulometry is an absolute method and thus no titer determination is necessary.

Coulometric titrations are carried out easily and quickly with the **851 Titrande**. The **852 Titrande** controls not only coulometric, but also volumetric Karl Fischer titration.

Bromine index

It is now possible to determine bromine indexes with the **851 Titrande** and the **852 Titrande**. No additional accessory parts are required for the measurements. The conventional coulometric titration cell and the generator electrode with diaphragm can also be used for bromine index determination. Only the anolyte and catholyte need to be adapted.

Automatic titration start

It can readily happen that the sample is injected into the titration vessel without the titration having been started beforehand. If this is the case, then the water in the

sample will be conditioned away and the measurement will need to be repeated. This will no longer be a problem for you with the **851 Titrande** or the **852 Titrande**. The instrument starts the titration automatically, as soon as the sample is added. This way, you save on reagents, sample and above all on precious time.

Coulometric and volumetric titrations

Should the water content of the samples be too high for coulometric determination, this will not be a problem for the **852 Titrande**. This instrument can determine samples with water contents ranging from a few micrograms to contents of 100% without difficulty.

Ordering Information

2.851.0010	851 Titrande with generator electrode with diaphragm
2.851.0020	851 Titrande with Touch Control and generator electrode with diaphragm
2.851.0110	851 Titrande with generator electrode without diaphragm
2.851.0120	851 Titrande with Touch Control and generator electrode without diaphragm
2.852.0050	852 Titrande with generator electrode with diaphragm
2.852.0060	852 Titrande with Touch Control and generator electrode with diaphragm
2.852.0150	852 Titrande with generator electrode without diaphragm
2.852.0160	852 Titrande with Touch Control and generator electrode without diaphragm

Options

2.800.0010	800 Dosino
2.801.0010	801 Stirrer
2.803.0010	803 TI Stand with stirrer and pump
2.900.0010	900 Touch Control
6.3032.120	Dosing Unit 2 mL
6.3032.150	Dosing Unit 5 mL
6.3032.210	Dosing Unit 10 mL
6.3032.220	Dosing Unit 20 mL
6.3032.250	Dosing Unit 50 mL
6.6056.241	tiamo ™ 2.4 Light CD: 1 license
6.6056.242	tiamo ™ 2.4 Full CD: 1 license
6.6056.243	tiamo ™ 2.4 Multi CD: 3 licenses



852 Titrande with 900 Touch Control

756/831 KF Coulometer

The Metrohm KF coulometers are suitable for precise water determination in the trace range (1 ppm to 10%). They come supplied with a selection of two different types of generator electrodes. The generator electrode without diaphragm requires only one reagent and is practically maintenance-free. The utilization of the generator electrode with diaphragm is preferred for the following applications: extremely low water content (<100 µg absolute water), utilization of ketone reagents or of a high proportion of solubility promoter (>10%).

With or without a printer – The choice is up to you! The 756 KF Coulometer comes equipped with a built-in thermal printer. You can, however, also connect an external printer or connect the instrument with a PC, just as you would with the 831 KF Coulometer.

You receive a complete titration cell and extensive accessories with all KF coulometers. The 728 Stirrer (magnetic stirrer) is included in the accessories of the KF coulometers with generator electrodes with diaphragm.

Arguments that convince:

- Live curve for early detection of possible side reactions
- Simple operation thanks to dialog in German, English, French, Spanish, Italian, Portuguese and Swedish.
- Selection of Expert or Routine mode
- Internal memory for up to 100 methods
- With two RS-232C (DB9) data interfaces for connecting balance, printer and PC
- Optional connection for PC keyboard and barcode reader
- Optional: Automatic reagent replacement via dosing unit and Dosino



756 KF Coulometer with 728 Stirrer

Ordering Information

2.756.0010	756 KF Coulometer with generator electrode with diaphragm
2.756.0110	756 KF Coulometer with generator electrode without diaphragm
2.831.0010	831 KF Coulometer with generator electrode with diaphragm
2.831.0110	831 KF Coulometer with generator electrode without diaphragm
2.831.2110	831 KF Coulometer and 860 KF Thermoprep

Options

2.140.0200	Impact printer CUSTOM DP40-S4N
2.700.0020	700 Dosino
2.703.0010	703 Ti Stand with stirrer and pump
2.728.0010	728 Stirrer without stand
6.5617.000	Equipment for reagent replacement

899 Coulometer

Small and compact

The 899 Coulometer is the smallest Metrohm coulometer. The magnetic stirrer is already built-in and a support rod can be dispensed with, thanks to the titration cell holder. The titration cell stands securely attached on the 899 Coulometer.

Automatic titration start

It can readily happen that the sample is added to the titration vessel without the titration having been started beforehand. In such cases, the conditioning continues to run until the reagent is once again titrated until it is dry. Recalculations are not possible and the determination must be repeated. This costs sample and valuable time.

The 899 Coulometer offers an automatic titration start. The titration starts automatically, as soon as sample is added to the titration vessel.

Flexible, thanks to accumulator

A Power Box can be obtained as an optional accessory for the 899 Coulometer. This ensures impressive flexibility. Determine the water content of your samples wherever you like.



899 Coulometer

Ordering Information

2.899.0010	899 Coulometer with generator electrode with diaphragm
2.899.0110	899 Coulometer with generator electrode without diaphragm
2.899.1010	899 Coulometer with generator electrode with diaphragm and Neo's USB thermal printer
2.899.1110	899 Coulometer with generator electrode without diaphragm and Neo's USB thermal printer
2.899.2110	899 Coulometer with generator electrode without diaphragm and 860 KF Thermoprep
2.899.3110	899 Coulometer with generator electrode without diaphragm and 885 Compact Oven SC

Options

2.141.0100	USB Thermal printer Neo's
6.2164.500	Power Box for 899
6.5406.000	Coulometric KF equipment, including generator electrode with diaphragm
6.5406.010	Coulometric KF equipment, including generator electrode without diaphragm

Manual KF Sample Preparation

Polytron PT 1300 D (2.136.0100)

Polytron PT 1300 D - Metrohm version
Homogenizer that can be controlled directly by *tiamo*[™]
or Touch Control.



KF Evaporator (2.136.0200)

The KF Evaporator is used for sample preparation in Karl Fischer titration by means of azeotropic distillation. As with the oven method, the water is separated from the sample matrix. Because the sample itself remains in the evaporation chamber, the titration vessel and the electrodes are not contaminated. Furthermore, unwanted side reactions and matrix effects are avoided.



860 KF Thermoprep (2.860.0010)

The 860 KF Thermoprep is designed for thermal sample preparation in Karl Fischer titration. Numerous substances cannot be analysed by direct Karl Fischer titration as they are not soluble, react with the Karl Fischer reagent or release their water only very slowly or not until heated to high temperatures. Using tightly sealed sample vials, the sample is inserted in the oven. The samples can be subsequently analysed by any volumetric or coulometric KF titrator.



Automated KF Sample Preparation

874 USB Oven Sample Processor

The 874 Oven Sample Processor opens up new possibilities for water content determinations in samples that either are insoluble, cause side reactions or cannot be introduced directly into the titration vessel for other reasons. These problems are avoided with the use of the oven method, because the water is separated from the difficult sample matrix.

Mode of operation of the oven technique

Each of the samples is introduced into the oven in tightly sealed sample vials. The water is released by the heating up of the sample and transferred into the KF cell with a flow of carrier gas. It is there that the Karl Fischer titration then takes place.

Sample preparation

Sample preparation for the oven technique is as simple as possible and consists solely of weighing the sample into the vial and then sealing it. In addition, the hermetic sealing of the vessels with septa reliably prevents the absorption of humidity from the ambient air.

Area of application

The oven method is suitable for liquid and solid samples and can be used with both volumetric and coulometric KF titrators.


The advantages of the oven method at a glance

- Reproducible analysis conditions for all samples, reflected in a markedly improved precision in the results
- Reduction of manual sample preparation to a minimum
- Considerable time savings
- No contamination of the oven or of the KF cell by the sample, thus precluding any carry-over or memory effects
- Improved release of water from the sample, because the carrier gas is not channeled over the sample, but rather directly through it
- Lower reagent consumption, as the titration solution needs to be replaced only rarely

874 USB Oven Sample Processor

- USB device – the 874 USB Oven Sample Processor is simply connected to a PC via USB port and recognized automatically.
- Optimum heating-up temperature – with the help of the temperature ramp, the optimum oven temperature can be determined for each sample.
- Reagent replacement – a 800 Dosino can be connected directly to an MSB connector of the changer and used together with a dosing unit for automatic replacement of the reagent.

Including **tiamo**TM full and extensive accessories, comprising 100 sample vessels, 100 septum caps, 1 pair of sealing pliers.

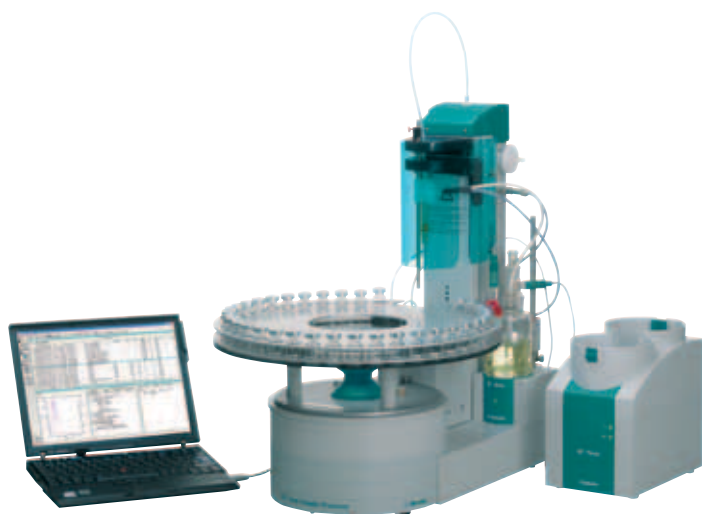

874 USB Oven Sample Processor with 851 Titrande

Ordering Information

- | | |
|------------|---|
| 2.874.0010 | 874 USB Oven Sample Processor with tiamo TM full |
| 2.874.0020 | 874 USB Oven Sample Processor customized with tiamo TM full |

Options

- | | |
|------------|--------------------------------|
| 6.1448.050 | Aluminum septum caps |
| 6.2419.000 | Sample glass, 6 mL, 1,000 pcs. |

885 Compact Oven Sample Changer

- Small space requirements – The instrument offers automation in the smallest possible space.
- Flexibility – The 885 Compact Oven Sample Changer can be operated with a coulometric or volumetric titrator.
- Simple operation – Only the oven temperature, the gas flow and the number of samples must be defined.
- Reusable sample vessels – After the analysis, sample vessels can be opened, cleaned and reused.

The 885 Compact Oven Sample Changer is used for thermal sample preparation in Karl Fischer titration. The samples are heated in the oven to a temperature of up to 250 °C. This causes the water to vaporize and be transported with a dry carrier gas into a titration cell in which the analysis takes place.

Area of application and principle of the oven method

The oven method is recommended for samples that release their water only at higher temperatures, for poorly soluble substances and those that react with the KF reagent.

The substance to be analyzed is placed in a tightly sealed sample vessel on the sample rack and heated up in the oven. A double needle pierces the septum and a dry flow of carrier gas transports the released water into the titration cell.

The advantage of the oven method lies in the fact that the sample itself does not enter the titration cell. This avoids the contamination of both the oven and titration cell, thus excluding both carry-over and memory effects that could falsify the results of the analysis.

Small space requirements

The name of the 885 Compact Oven Sample Changer explains its purpose: The instrument offers automation in a minimum amount of space.

Great flexibility

Depending on the sample, Karl Fischer titration can be either coulometric or volumetric. No matter which method is used – the 885 Compact Oven Sample Changer can be operated with all stand-alone KF titrators with sample table.

Simple operation

The instrument is controlled using the integrated keypad. Only the oven temperature and the gas flow must be defined and the number of the samples to be determined must be established.

Reusable sample vessels

Screw-cap vials are used with the 885 Compact Oven Sample Changer. After the measurement, these sample vessels can be opened, cleaned and subsequently reused without difficulty. Only the septum must be replaced after it has been pierced.



885 Compact Oven Sample Changer

Ordering Information

2.885.0010 885 Compact Oven Sample Changer

Options

6.1448.077 Septum

6.2141.340 Remote cable 885 - Remote Box MSB

6.2148.010 Remote Box MSB

KF Automation

Automated coulometric KF titrations (MATi 04)

MATi 4 is a fully automated system for coulometric Karl Fischer titrations with high sample throughput. Up to 160 samples in 6 mL vials can be placed on the sample rack of the Sample Processor. The sample is pipetted into an external coulometric cell and then titrated there. The system is controlled by means of the **tiamo™** titration software.




Automated volumetric KF titrations (MATi 10)

Fully automated system for volumetric Karl Fischer water content determination in up to 24 samples. The system is controlled with **tiamo™** and consists of an 814 USB Sample Processor, a 901 Titrand and extensive accessories. The samples are weighed out into the beakers, sealed to protect against humidity and placed on the rack. Before the actual titration, they are dissolved in a KF working medium, after which the water content is titrated.



Automated volumetric KF titration including sample preparation (MATi 11)

Fully automated system for volumetric Karl Fischer water content determination in up to 53 samples. This system is controlled with **tiamo™** and consists of an 815 Robotic USB Sample Processor XL, a 901 Titrand and extensive accessories. The samples are pulverized in a short time with the Polytron and the water they contain is released. Even samples of poor solubility, e.g., tablets, can be analyzed without difficulty with this method. The use of solubility promoters can be avoided in this way.

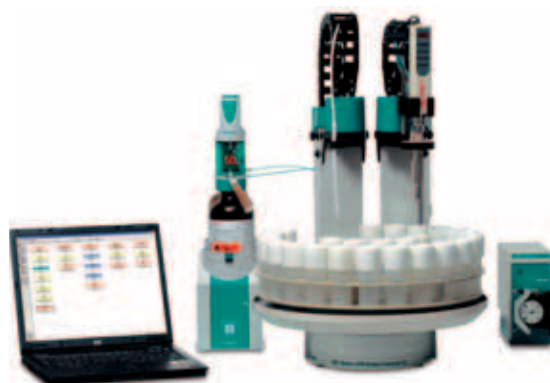

KF Gas Analyzer

875 KF Gas Analyzer

- Complete system with durable components for high flexibility and for pressures up to 40 bar
- Separation of the gas-carrying system from the electronics and the power supply
- Input filter for avoiding the introduction of particles by the sample
- Integrated vaporizer for liquefied gases
- Oil filter for removing oil residue
- Precise gas measurement with mass flow measurement instrument
- Automated analysis process
- Predefined analysis methods
- All components are integrated in a single housing

The KF Gas Analyzer is a robustly constructed analysis system for routine water content determination in liquefied and permanent gases.

The system is controlled with **tiamo**[™] and is comprised of one operating unit (TFT monitor) and an analysis module. The analysis module is fitted with the gas path, a titration vessel and a coulometer. This makes it possible to perform all analysis steps fully automatically.


The system was designed for water content determination in gases in accordance with Karl Fischer and is also suitable for very low water content determinations.

Application examples

Water content determination in various liquefied gases

- Propane, propene, LPG, butane, butene, butadiene
- Dimethyl ether
- Methyl chloride, ethyl chloride, vinyl chloride
- CFC, HFC, CHC, fresh and used refrigerants with chiller oil contents

Water content determination in permanent gases such as natural gas

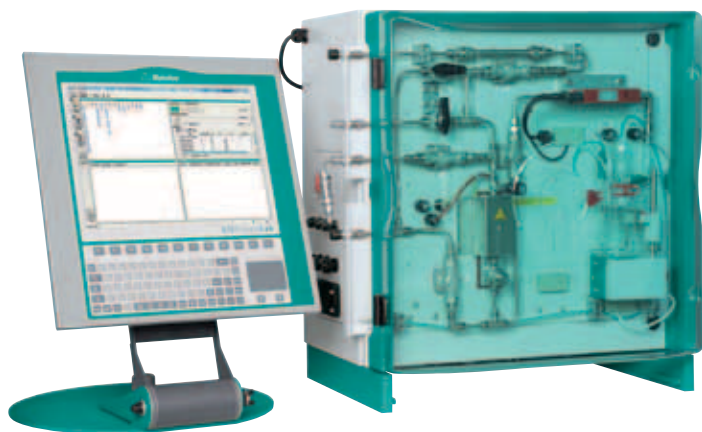

875 KF Gas Analyzer

Ordering Information

- 2.875.9020 KF Gas Analyzer with TFT monitor
- 2.875.9050 KF Gas Analyzer without TFT monitor

Options

- 6.7209.000 KF Gas Analyzer equipment for reagent replacement and adding methanol
- 6.7209.010 KF Gas Analyzer equipment for rinsing with solvent



Dosing devices



Dosing devices

Dosing, pipetting and manual titration	54
The Dosimats at a glance	54
865 Dosimat plus	55
876 Dosimat plus – 876 Manual Titrator	56
Intelligent Liquid Handling	57
846 Dosing Interface	57

Dosing, pipetting and manual titration

The Dosimats at a glance

	876 Dosimat plus	876 Manual Titrator plus	865 Dosimat plus
Steps per cylinder volume	10 000 Pulses	10 000 Pulses	10 000 Pulses
Printer connection (USB)	yes	yes	yes
Remote Interface	yes	yes	yes
Balance Connection via RS232	yes (6.2148.030)	yes (6.2148.030)	yes (6.2148.030)
Intelligent Exchange unit	yes	yes	yes
Push Button Cable	yes	yes	yes
Manual Dosing (DOS)	yes	yes	yes
Manual Titration	yes	yes	yes
Extended Dosing (XDOS)	yes	yes	yes
Content Dosing (CNT D)	–	–	yes
Liquid Transfer (LQT)	–	–	yes
Tandem Dosing (with 805 Dosimat)	yes	yes	yes
Including 801 Magnetic Stirrer and Stand	optional	yes	optional
Remote Control via PC	yes	yes	yes



865 Dosimat plus

Universal dispensing unit for titration and dosing tasks in the laboratory. Including push-button cable for manual dispensing control and 6.3026.220 exchange unit (20 mL).

A multitude of instruments can be connected at the USB interface of the Dosimat plus, even a number of them simultaneously when a USB hub is used (keyboard, mouse, USB compact printer or USB DIN A4 printer, USB Memory Stick for methods and data backup). The optional 6.2148.030 USB/RS-232 adapter box enables the connection of laboratory balances and operation with a computer.

With its four dosing modes, the Dosimat plus offers a multitude of applications:

DOS (Dosing)

Dosing at the press of a button, particularly suitable for performing manual titrations with indicator. A result can be calculated automatically from the dosed volume and a result report can be printed out. Different calculation variables can be defined in advance as parameters.

XDOS (Extended Dosing)

Fixed volume dosing: The volume and the dosing rate are specified.

Time-controlled dosing: The volume and the time are specified.

Dosing according to dosing rate: The dosing rate and the time are specified.

If continuous dosing without interruption is required, then the 865 Dosimat plus can be operated together with an 805 Dosimat in tandem mode.

CNT D (Content dosing)

This mode is suitable for the preparation of standard and other solutions. The 865 Dosimat plus automatically determines the volume of the solvent to be dosed on the basis of the sample size of the starting substance (solid or stock solution) and the specified target concentration. A report containing all of the relevant data concerning the solution that was prepared can be printed out after the dosing.

LQT (Liquid transfer)

This mode is suitable for the pipetting and diluting of liquids.



865 Dosimat plus with 801 Magnetic Stirrer (optional)

Ordering Information

2.865.0010 865 Dosimat plus

876 Dosimat plus – 876 Manual Titrator

Metrohm Dosimats make routine Liquid Handling easier. They are used to accomplish a wide variety of dosing and Liquid Handling tasks in laboratories around the world. The new Dosimats can be used as autonomous, manually operated instruments or they are used as automatic dosing devices for Titrino/Titrino plus titrators.

The 876 Dosimat plus is suitable for hand titrations and dosings. A push-button cable for manual dispensing control and a 20 mL exchange unit are supplied with the Dosimat plus.

The 876 Manual Titrator with flat stopcock switching and refilling is used for result calculations for titration with color indicator. The instrument is also supplied with a push-button cable for manual dispensing control, a 20 mL exchange unit and a magnetic stirrer.

A multitude of instruments can be connected at the USB interface of the Dosimat plus and Manual Titrator, even a number of them simultaneously when a USB hub is used (keyboard, mouse, USB compact printer or commercially available USB DIN A4 printer, USB Memory Stick

for methods and data backup). The optional 6.2148.030 USB/RS-232 adapter box enables the connection of laboratory balances and remote control with a PC. With its two dosing modes, the Dosimat plus and the Manual Titrator are outstandingly suitable for classic laboratory dosing tasks.

DOS (Dosing)

Dosing at the press of a button, particularly suitable for performing manual titrations with indicator. A result can be calculated automatically from the dosed volume and a result report can be printed out. Different calculation variables can be defined in advance as parameters.

XDOS (Extended Dosing)

Fixed volume dosing: The volume and the dosing rate are specified.

Time-controlled dosing: The volume and the time are specified.

Dosing according to dosing rate: The dosing rate and the time are specified.

If continuous dosing without interruption is required, then the 876 Dosimat plus can be operated together with an 805 Dosimat in tandem mode.



876 Manual Titrator

Ordering Information

- 2.876.0010 876 Dosimat plus
- 2.876.0110 876 Manual Titrator plus

Options

- 2.801.0040 801 Stirrer with stand
- 2.802.0040 802 Stirrer (propeller stirrer) for 804 Ti Stand
- 2.804.0010 804 Ti Stand without stand rod
- 2.804.0040 804 Ti Stand with stand
- 2.805.0010 805 Dosimat
- 6.3026.110 Exchange Unit 1 mL
- 6.3026.150 Exchange Unit 5 mL
- 6.3026.210 Exchange Unit 10 mL
- 6.3026.220 Exchange Unit 20 mL
- 6.3026.250 Exchange unit 50 mL

Intelligent Liquid Handling

846 Dosing Interface

The 846 Dosing Interface can be seamlessly incorporated as a system component and control instrument into a Metrohm Titrand system. The interface is operated with a Touch Control or from a PC with *tiamo*[™].

Comprehensive Liquid Handling

Basic operations of everyday laboratory work such as pipetting, transferring, dosing, dispensing and diluting become child's play thanks to the innovative Liquid Handling functionality of the Dosing Interface in connection with the 800 Dosino. The system guarantees maximum accuracy and precision in the range of 10 µL to 100 mL, i.e. across no fewer than four orders of magnitude.

The control device has four MSB connectors (MSB = Metrohm Serial Bus) at which auxiliary and peripheral devices can be operated. Numbered among these are one dosing drive each (800 Dosino or 805 Dosimat), one stirrer or titration stand, one Remote Box, etc. Two USB connectors continue to be available through which such instruments as printer, balances, keyboard, barcode reader, a USB Sample Processor or other control devices can be connected.



846 Dosing Interface with 900 Touch Control

Ordering Information

2.846.0010	846 Dosing Interface
2.800.0010	800 Dosino

Options

2.801.0040	801 Stirrer with stand
6.2061.010	Bottle holder for Dosinos
6.2065.000	Stacking frame for 846 Dosing Interface, 856 Conductivity Module, 867 pH Module
6.3032.120	Dosing Unit 2 mL
6.3032.150	Dosing Unit 5 mL
6.3032.210	Dosing Unit 10 mL
6.3032.220	Dosing Unit 20 mL
6.3032.250	Dosing Unit 50 mL



Automation in titration



Automation in titration

Introduction to automation	62	Automation peripheral devices	80
Automation in titration	62	Membrane pumps	80
Overview of sample changers	63	Peristaltic pumps	81
		849 Level Control	82
Sample Changer	64	731 Relay Box	83
869 Compact Sample Changer	64	786 Swing Head	84
898 XYZ Sample Changer	65	741 Magnetic Stirrer	85
		802 Stirrer	85
USB Sample Processors	66		
814 USB Sample Processor	66		
815 Robotic USB Sample Processor XL	67		
864 Robotic Balance Sample Processor TAN/TBN	68		
Titrosampler	69		
862 Compact Titrosampler	69		
855 Robotic Titrosampler	70		
Titration systems	71		
Introduction – Automated systems	71		
848 Titropackage plus	72		
MATi systems	73		
Fully automatic water analysis	73		
Automated TAN/TBN analysis	73		
Nonaqueous titrations	73		
Automatic titration of acids and bases for up to 12 samples	73		
Automated titration system for up to 28 samples	74		
Automated pipetting and titration system for up to 100 samples	74		
Automated COD determination	74		
Fully automated determination of the permanganate index, according to DIN EN ISO 8467	74		
862 Compact Titrosampler	75		
Robotic Analyzer packages	76		
Robotic Chloride Analyzer	76		
Robotic Acid-Base Analyzer	76		
Robotic TAN/TBN Analyzer	76		
Robotic Fluoride Analyzer	76		
Robotic Transfer Analyzer	77		
Sample preparation systems	78		
An overview of sample preparation	78		
Robotic Soliprep	79		

Introduction to automation

Automation in titration

The automation of potentiometric measurement methods has gained enormously in importance as it becomes ever less frequently the case that simple determinations are sufficient. In contrast to purely manual determination, the fully automatic alternative is very precise, safe and time-saving.







With large **numbers of samples**, the thought of automation of the analysis that is always the same quickly presents itself, particularly since qualified personnel can be utilized more efficiently when the routine is taken over by a completely automated system. Even in the case of smaller series or with many different analyses, automation can help achieve more rapid and more reproducible results.

A uniform **sample preparation** that can be guaranteed only with a completely automated system ensures that the results will continue to be identical – independent of the user – even over long periods of time. Typical preparatory steps from everyday lab work such as Liquid Handling (pipetting, transferring), dilution, addition, tempering, degassing, pulverization, filtration, filling and much more can proceed just as automatically as the subsequent analytical determination.

One aspect not to be neglected is that of safety in the laboratory. The frequent handling of typical laboratory equipment (pipettes, burets, etc.) and the exposure to aggressive chemicals requires the complete concentration of the laboratory employee. When automated systems are used with sample preparation, the contact with hazardous substances and solvents is minimized, thus massively enhancing occupational safety.

Metrohm offers a large selection of instruments for the automation of your analysis, including sample preparation. On the following pages, you will learn more about the various sample changers and the completely preconfigured analysis systems.

Overview of sample changers

						
	862 Compact Titrosampler	869 Compact Sample Changer	814 USB Sample Processor	815 Robotic USB Sample Processor XL	855 Robotic Titrosampler	864 Robotic Balance Sample Processor
Integrated measuring input	yes	–	–	–	yes	–
Integrated balance	–	–	–	–	–	yes
Work stations	1	1	1 / 2	1 / 2	1	2
Automatic rack recognition	yes	yes	yes	yes	yes	yes
Exchangeable racks	–	–	yes	yes	yes	yes
Titration/measurement directly on the rack	yes	yes	yes	yes	yes	yes
Standard racks	11 x 120 mL	11 x 120 mL	12 x 250 mL 14 x 200 mL 16 x 150 mL 22 x 120 mL 24 x 75 mL	28 x 250 mL 28 x 200 mL 34 x 150 mL 59 x 120 mL 100 x 75 mL 160 x 6 mL 228 x 11 mL	28 x 250 mL 28 x 200 mL 34 x 150 mL 59 x 120 mL 100 x 75 mL 160 x 11 mL 228 x 11 mL	20 x 120 mL
Thermostated racks	–	–	–	yes	yes	–
Beaker sensor	–	–	yes	yes	yes	yes
Splash protection	yes	yes	yes	yes	yes	yes
Drip pan	–	–	yes	yes	yes	yes
Max. number internal pumps	–	–	2 / 4	2 / 4	2	–
Max. number external pumps	2	2	2 / 4	2 / 4	1	4
Connector Swing Head	–	–	1 / 2	1 / 2	1	2
External positions	–	–	4 / 8	4 / 8	4	8
Pipetting / Sample transfer	–	–	yes	yes	yes	yes
Stirrer connector	1	1	1 / 2	1 / 2	1	2
Connector MSB	–	–	3	3	3	3
Connector Remote	yes	yes	optional	optional	optional	optional
Connector USB	–	–	2	2	2	2
Connector Mini-USB	yes	yes	–	–	–	–
Stand-alone	yes	yes	optional	optional	optional	–
tiamo™	–	–	yes	yes	yes	yes

Sample Changer

869 Compact Sample Changer

- Inexpensive automation
- Space-saving
- Various method templates
- Simple operation
- A total of 12 positions
- Live display

The 869 Compact Sample Changer offers automation in a minimum amount of space.

The 869 Compact Sample Changer offers the rapid and simple automation of Titrino and Titrino plus applications. For multiple determinations and **small sample series**, this sample changer is just the right choice. A wide variety of titrations can be performed fully automatically in a total of 12 positions and the electrode can be cleaned and/or conditioned between the determinations. In order to keep the consumption of titrant and solvents as low as possible, slender sample beakers are used as standard equipment that enable low-waste and rapid titration with even small volumes.



869 Compact Sample Changer

Thanks to the large and clearly organized **live display**, the current status of the sample series can be recognized directly and important samples can be given preferential analysis at any time. In light of the fact that laboratory space is expensive and rare, the compact sample changer requires no more support surface than that of a commercially available laboratory balance.

Various **method templates** can be used as the basis for creating and storing application-specific methods. Only four parameters need to be set on the 869 Compact Sample Changer for this purpose. In addition, the methods can also be printed out or saved electronically via USB (OTG) connector. Communication between Compact Sample Changer and Titrino / Titrino plus takes place via remote signals with an additional control box or PC being required.

The titration head of the sample changer offers space for an 802 Stirrer propeller stirrer and two additional electrodes. The propeller stirrer can be connected directly to the instrument and is also monitored by it. Titrant and auxiliary reagent can be added with the buret tips that have already been inserted. The 869 Compact Sample Changer can be equipped with rinsing and aspiration pumps upon request. Despite its inexpensive price, no corners were cut with respect to **safety** with the 869 Compact Sample Changer. The safety shield protects the user against inadvertent contact with chemicals.

Ordering Information

2.869.0010 869 Compact Sample Changer

898 XYZ Sample Changer

- Simple automation for high numbers of samples
- Time savings thanks to high speed
- Measuring and titration directly in the sample beaker
- Precise and reproducible results


XYZ Sample Changer with one workstation, one membrane pump and rinsing station for the automatic processing of routine samples in large numbers. The control takes place via computer operation using the **tiamo™** titration software.

Time savings and improved operating sequences

The advantages of a sample changer lie not only in the time savings for the laboratory personnel: Automatic systems control operating sequences, prevent errors and thus improve reproducibility and accuracy. Independent of the time of day, the system works through the prepared samples (automatic sample preparation, Liquid Handling or sample processing) and guarantees thereby the complete traceability of the individual steps.

The 898 XYZ Sample Changer convinces with its speed and the number of samples that can be processed without supervision. Two sample racks with 41 x 120 mL beakers or 24 x 250 mL beakers each can be fitted on the 898 XYZ SC and processed continuously there. As soon as the processing of the first sample rack has been completed, it can be replaced while operations are running.

Whereas beakers, sample racks, titration head and tubing are already included in the package, stirrers, propeller stirrers and Ti Stand (if needed) must be ordered separately in accordance with the titrator.

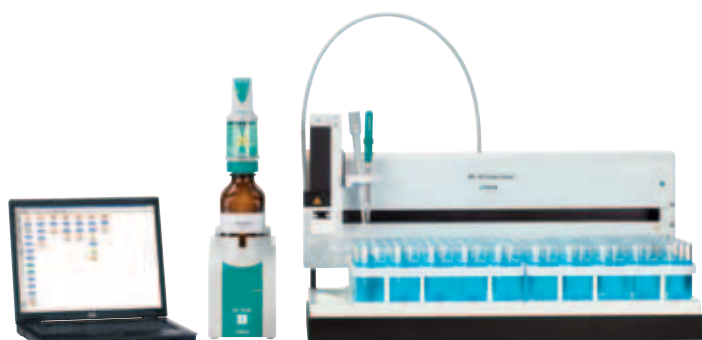

898 XYZ Sample Changer

Ordering Information

2.898.0110	898 XYZ Sample Changer 82 x 120 mL
2.898.0210	898 XYZ Sample Changer 48 x 250 mL

USB Sample Processors

814 USB Sample Processor

In today's world, single determinations are simply no longer enough!

In modern-day laboratories single determinations no longer meet the requirements. Each and every result has to be confirmed by multiple determinations in order to meet the **tough quality standards**. An „automatic“ titrator without sample changer is therefore basically just a semiautomatic titrator because it is not able to carry out a double or threefold determination by itself: each titration requires the user to take action, which is both tedious and time-consuming.

The benefits of a sample changer are not just found in the time saved by lab personnel: automated systems control operation sequences and thus improve **reproducibility and accuracy**. Errors can be reduced to a minimum. The system processes the prepared samples irrespective of the time of day. No matter whether automatic sample preparation, liquid handling or sample processing - the 814 USB Sample Processor masters everything that used to be the exclusive domain of laboratory robots.

Thanks to its compact design, even complex tasks can be carried out reliably on the smallest possible footprint. Depending on the sample matrix, the titrated sample solution is aspirated and the titration equipment is rinsed using **membrane or peristaltic pumps**. These are either mounted already inside the instrument or available as peripheral devices.

Depending on the user's preference, the 814 USB Sample Processor can be controlled by **Touch Control**, the **tiamo™** titration or the **MagIC Net** chromatography software. The method examples provided make creating your own methods perfectly easy.



814 USB Sample Processor with sample rack for 12 x 250 mL

Ordering Information

2.814.0010	814 USB Sample Processor (1T/1P)
2.814.0020	814 USB Sample Processor (1T/2P)
2.814.0030	814 USB Sample Processor (1T/0P)
2.814.0110	814 USB Sample Processor (2T/2P)
2.814.0120	814 USB Sample Processor (2T/4P)
2.814.0130	814 USB Sample Processor (2T/0P)

815 Robotic USB Sample Processor XL

Minimum effort with maximum sample throughput!

In view of the **large number of samples** and ever more elaborate preparation steps, the use of robots is becoming ever more important, even in analytical laboratories. The larger the number of steps per sample that must be completed, the more their professional automation pays off. It has been a long time since this merely involved switching from one beaker to the next in order to analyze the sample – more and more it is the simplification of the entire sample processing, from the preparation to the multiple determination, that is demanded.

Reproducibility and accuracy are the alpha and omega in analysis and are thus numbered among the main requirements of automation. Robotic Sample Processors make child's play of the basic operations of modern automation, e.g., **pipetting, transferring, aliquoting, dosing and dispensing**.

The use of the 786 Swing Head ensures that a **maximum number of sample vessels** can always be posi-

tioned on the rack, so that series as large as possible can be processed. Depending on the application and the vessel size used, this maximum is between 28 and 228 positions (standard racks).

Thanks to the compact design, even more complex tasks can be managed reliably. **Parallel processing** of the samples is accomplished easily and conveniently with the Robotic Sample Processor XL. While the pipetted sample volume is titrated at an external workstation (optional), the pH of the prepared samples can also be determined, for example, or the next sample can already undergo preparation. This means the time per analysis is reduced to a minimum.

Depending on the requirements, the 815 Robotic USB Sample Processor XL can be operated using **Touch Control**, the **tiamo™** titration software or the **MagIC Net** chromatography software. Method development is child's play with the example methods supplied.



815 Robotic USB Sample Processor XL

Ordering Information

2.815.0010	815 Robotic USB Sample Processor XL (1T/1P)
2.815.0020	815 Robotic USB Sample Processor XL (1T/2P)
2.815.0030	815 Robotic USB Sample Processor XL (1T/0P)
2.815.0110	815 Robotic USB Sample Processor XL (2T/2P)
2.815.0120	815 Robotic USB Sample Processor XL (2T/4P)
2.815.0130	815 Robotic USB Sample Processor XL (2T/0P)

864 Robotic Balance Sample Processor TAN/TBN

- Fully automatic weighing of the sample
- High-end analyzer with a minimum footprint
- Robotic USB Sample Processor - proven technology
- Sample preparation and analysis in one system
- Saves time by taking over routine tasks
- Intelligent liquid handling - transferring, diluting and more
- Reliable, robust and safe
- Attractive price
- Control software that leaves nothing to be desired

System for the fully automatic preparation and analysis of petrochemical products that need to be weighed in, diluted and titrated.

System includes the following instruments:

- 1 x 864 Robotic Balance Sample Processor XL
- 1 x 905 Titrando
- 3 x 800 Dosino
- 1 x 786 Swing Head
- 1 x 786 Swing Head strengthened
- 1 x 802 Stirrer
- 1 x 843 Pump Station (Peristaltic)

The 864 Robotic Balance Sample Processor TAN/TBN offers fast and convenient sample preparation combined with **the analysis of petrochemical products** in one system.

The sample is placed in a beaker on the sample rack and an aliquote of it is pipetted and weighed into the titration beaker fully automatically. After **sample transfer and weighing**, the sample is diluted with solvent. The TAN or TBN value is then determined by titration. After the analysis the titration beaker is emptied and the titration equipment is cleaned directly inside the beaker.

The sample rack can accommodate 20 sample and titration beakers (6.1459.300) each as well as 20 pipetting tips (6.1562.240) for sample transfer. These 10 mL tips are picked up, filled and stripped off after weighing so that **cross-contamination-free sample transfer** is absolutely guaranteed. Time and amount of work per sample is minimized. The only thing that needs to be ensured is that enough sample is in the beaker.

The combined automation of sample preparation and analysis in a single system increases **reproducibility** and **accuracy** of results as the sample is weighed in where it will be analysed. If necessary, the equipment can be cleaned more intensely by using an additional external rinsing station combined with a second 843 Pump Station.

The complete preparation and analysis system is controlled by the approved titration software **tiamo™**. Each preparation step (including the sample amount weighed in) is documented in a database as are the titration results for each single sample.



864 Robotic Balance Sample Processor TAN/TBN

Ordering Information

2.864.1130 864 Robotic Balance Sample Processor TAN/TBN

Titrosampler

862 Compact Titrosampler

The 862 Compact Titrosampler – **titrator and sample changer** in one – is a completely automated titration station with the support surface of a commercially available analytical balance.

A wide variety of analyses can be performed fully automatically in a total of 12 positions and the electrodes can be cleaned and/or conditioned between the determinations. The titration curve is directly in view thanks to the large, clearly organized **Live Display** and the current status of the sample series is recognizable at once. Pressing samples can be given priority analysis at any time. „Plug & Play“ functionality of intelligent dosing unit, stirrer and USB printer, a high-precision measuring input, operation per mouse click and a variety of dialog options – this combination device leaves nothing to be wished for.

Highest degree of precision thanks to the new measuring input: Just as is the case with the high-end Titrande titrator, the new Compact Titrosampler is also equipped with a high-resolution measuring input which guarantees results with the greatest of precision. A multi-

tude of instruments can be connected to the USB interface of the Compact Titrosampler, even a number of them at once when a USB hub is used:

- Numerical keypad
- USB compact printer
- Commercially available USB DIN A4 printer
- USB Memory Stick for methods and data backup



862 Compact Titrosampler with printer

Ordering Information

2.862.0010	862 Compact Titrosampler
2.862.0110	862 Compact Titrosampler with printer

855 Robotic Titrosampler

The most discrete titrator in the world – invisible and yet so flexible.

The 855 Robotic Titrosampler opens up a new dimension in automation. The successful **combination** of high-performance titrator and perfect laboratory automation at the robot level covers an extensive spectrum of applications. Thanks to this combination of automation and titration, up to 40% of the space usually required can be dispensed with – and this with identical functionality and unchanging flexibility.

The more demanding the application, the more work steps there are that are required prior to the actual determination. The time-consuming **sample preparation** can be left to the Robotic Titrosampler. Whether it be pipetting, transferring or simply diluting with solvent – there is practically no limit to what is possible. With up to three buret connections integrated in the instrument, the Robotic Titrosampler offers sufficient latitude for Liquid Handling tasks.

A high-performance titrator based on the **proven Titrando technology** is already integrated in the Robotic Titrosampler. With the **accuracy and precision** of the Titrando, the Robotic Titrosampler is also equipped with the STAT mode in addition to the usual titration modes. Dynamic (DET) and monotonic (MET) titration, endpoint titration (SET), enzymatic and pH-Stat titration (STAT), measurement with ion-selective electrodes (MEAS CONC) and Liquid Handling (LQH, DOS) are child's play with the Robotic Titrosampler.

With the multitude of combination options and in view of the many different applications that are processed nowadays in laboratories, it is imperative that the retraceability of each individual sample be guaranteed. With its connectors for intelligent dosing units, the 855 Robotic Titrosampler offers **complete documentation** of your analysis.

The control can be accomplished either using the handy **Touch Control** or with the state-of-the-art **tiamo™** titration software.



855 Robotic Titrosampler „Basic“

Ordering Information

2.855.0010	855 Robotic Titrosampler „Basic“ (1T/1P)
2.855.0020	855 Robotic Titrosampler „Basic“ (1T/2P)

Titration systems

Introduction – Automated systems

Profit from more than 60 years of experience!

Metrohm offers much more than only a wide variety of different individual instruments out of which you can select according to your requirements. Complete systems have been assembled on the basis of the application experiences of the last 60 years that are targeted to fulfil various requirements. Select your automated Metrohm laboratory instruments quickly and easily – with the assurance that we have already thought of everything.

848 Titropackage plus

The compact and inexpensive system for the automation of potentiometric analyses in the smallest possible space! The combination of routine titrator and very compact sample changer requires exceptionally little space and can be put into operation in a very small amount of time.

MATi systems

These systems (MATi = Metrohm Automated Titration) are tailored to various standard applications and offer a maximum of convenience and flexibility. More than ten different, fully automated systems offer the perfect basis for the determination of your samples.

Compact Titrosampler packages

The Compact Titrosampler packages each covers one standard application – and that with minimum space requirements. The „Food/Beverage“ and „Salt“ packages are furnished with the accessories required for the application, so that you can begin working immediately. Just install and go.

Robotic Analyzers

The Robotic Analyzer family is comprised of various packages, each of which covers a standard application. Each of these packages offers you the perfect framework for the solution of your application. The centerpiece is always the unique 855 Robotic Titrosampler, the space-saving combination of a titrator installed in the sample changer. Depending on the application, this titrating analyzer is equipped with the accessories tailored to your application. You receive exactly what you need, no more and no less.

Because of the great flexibility of Metrohm automation, the systems can be adapted and expanded according to customer specifications upon request.

848 Titropackage plus

Compact and inexpensive system for the automation of potentiometric determinations in the smallest possible space. Comprised of:

- 1 x 848 Titrino plus
- 1 x 802 Stirrer
- 1 x 869 Compact Sample Changer

The 848 Titropackage plus contains everything required to enable rapid installation and direct entry into working with the system. A large number of pre-defined titration methods, combined with very simple operation, permits immediate use.

Titrino plus

The Titrino plus, Metrohm's new entry class in the area of potentiometric titration, is particularly attractive due to its practically unbelievable price-performance ratio. A large live display with titration curve, „Plug & Play“ functionality of exchange unit, stirrer and USB printer, a high-precision measuring input, operation per mouseclick – the Titrino plus offers considerably more than you would ever expect in this price segment. With its operating

dialog, which is tailored to routine users, the Titrino plus instruments are so simple to operate that only brief orientation periods are required. Their robustness also makes them the ideal titrators for routine determinations in everyday laboratory operations.

Compact Sample Changer

For multiple determinations and small sample series, this sample changer is just the right choice. A wide variety of titrations can be performed fully automatically in a total of 12 positions and the electrode can be cleaned and/or conditioned between the determinations. In order to keep the consumption of titrant and solvents as low as possible, slender sample beakers are used as standard equipment that enable low-waste and rapid titration with even small volumes. Thanks to the large and clearly organized live display, the current status of the sample series can be recognized directly and important samples can be given preferential analysis at any time. In light of the fact that laboratory space is expensive and rare, the compact sample changer requires no more support surface than that of a commercially available laboratory balance.



848 Titropackage plus

Ordering Information

- | | |
|------------|--------------------------------|
| 2.848.0110 | 848 Titropackage plus |
| 2.848.0120 | Titropackage plus with printer |

MATi systems

Fully automatic water analysis (MATi 01)

PC-controlled, fully automatic water analysis system with a rapid measurement system for the precise sample transfer of 100 mL samples. After the conductivity measurement, pH value, alkalinity and Ca/Mg content are determined in an external cell. Up to 59 samples can be placed on the rack. The control of this system is handled by the proven **tiamo™** titration software.



Automated TAN/TBN analysis (MATi 02)

PC-controlled, fully automatic analysis system for the direct determination of TAN or TBN values in mineral oil products in series of up to 59 samples. The analysis is carried out in accordance with ASTM standards D664 and D2896. The system is noteworthy for its special resistance to the solvents used in these applications. The data acquisition and the complete control of the system takes place via the proven **tiamo™** titration software.



Nonaqueous titrations (MATi 03)

Direct nonaqueous titration of pharmaceutical active ingredients and other substances in series of up to 59 samples. The system is noteworthy for its special resistance to organic solvents. The control of this system is handled by the proven **tiamo™** titration software, that can also be provided in an FDA-compliant version upon request.




Automatic titration of acids and bases for up to 12 samples (MATi 06)

Fully automatic system for potentiometric titration of acids and bases in series of up to 12 samples. The titration is carried out directly in the beaker on the rack. Afterwards, the electrode is cleaned automatically using the membrane pumps built into the sample changer and the titration beaker is emptied. The control of this system is handled by the user-friendly **tiamo™** titration software.



Automated titration system for up to 28 samples
(MATi 07)

Fully automated system for the performance of potentiometric titrations such as acid/base, Redox and classic halogenide titration in series of up to 28 samples. The system is controlled with the **tiamo™** titration software. At the end of the determination, the electrode and buret tips are cleaned automatically using the Pump Station and the beaker is emptied.

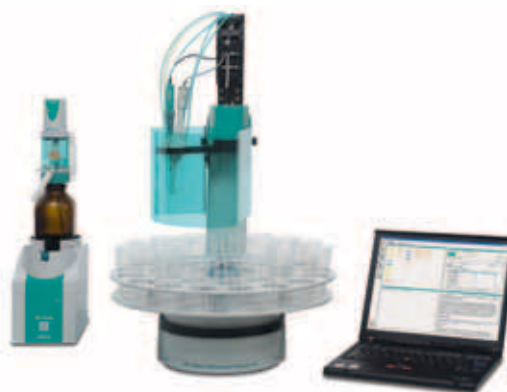

Automated pipetting and titration system for up to 100 samples (MATi 08)

Automated system for the performance of potentiometric titrations on acids and bases in up to 100 samples. The sample is pipetted out of the beaker into the external titration vessel, after which a completely automatic determination is carried out. After the titration, the external vessel is cleaned thoroughly using the membrane pumps built into the Sample Processor. The control of this completely automatic analysis system takes place using the proven **tiamo™** titration software.



Automated COD determination (MATi 12)

Automatic system for potentiometric titration of COD samples in series up to 21 samples. The titration is carried out directly in the reaction vessel on the rack. Afterwards, the electrode is cleaned automatically by means of the membrane pump built into the sample changer and the reaction vessel is emptied. The control of this system is handled by the user-friendly **tiamo™** titration software.



Fully automated determination of the permanganate index, according to DIN EN ISO 8467
(MATi 13)

Automated system for the determination of the permanganate index in accordance with DIN EN ISO 8467. Up to 24 samples can be placed on the rack and processed within one series. The sample is pipetted from the sample beaker into the external titration cell and analyzed completely automatically in accordance with the requirements of the DIN standard. The system is controlled by the **tiamo™** titration software.



862 Compact Titrosampler

- Compact and inexpensive automated titration instrument
- Simple installation and operation
- Intelligent dosing unit and monitoring of the titrant
- Ready for immediate use
- Maximum precision thanks to high-resolution measuring input
- Live curve
- USB compact printer as option

The 862 Compact Titrosampler is an instrument for the determination of dynamic (DET) and monotonic (MET) titrations with automatic equivalence point finding and endpoint titrations (SET) in a very small space. The combination of titrator and sample changer in a single instrument requires no more support surface than that of a commercially available analytical balance. Thanks to the USB printer, the results can be documented directly and clearly.

A wide variety of analyses can be performed fully automatically in a total of 12 positions and the electrodes can be cleaned and/or conditioned between the determinations. The titration curve is directly in view thanks to the large, clearly organized Live Display and the current status of the sample series is recognizable at once. Pressing samples can be given priority analysis at any

time. „Plug & Play“ functionality of intelligent dosing unit, stirrer and USB printer, a high-precision measuring input, operation per mouse click and a variety of dialog options – this combination device leaves nothing to be wished for.

Maximum precision thanks to the new measuring input

Just as is the case with the high-end titrator Titrande, the Compact Titrosampler is also equipped with a high-resolution measuring input which guarantees results with the greatest of precision.

USB interface

A multitude of instruments can be connected to the USB interface of the Compact Titrosampler, even a number of them at once when a USB hub is used:

- Keyboard or mouse
- USB compact printer or commercially available USB DIN A4 printer
- USB Memory Stick for methods and data backup

862 Food/Beverage Compact Titrosampler

The 862 Food/Beverage Compact Titrosampler is a compact and inexpensive instrument for the automatic performance of most potentiometric analyses required in the food industry. Equipped with extensive accessories, the 862 Food/Beverage Compact Titrosampler is ready for immediate use.

862 Salt Compact Titrosampler

The 862 Salt Compact Titrosampler is comprised of a complete package for the analysis of chloride in a very wide variety of samples. The accessories included are tailored precisely to this application, thus enabling not only simple and rapid installation but also clearly organized documentation of the results with the USB printer that is included.



862 Food/Beverage Compact Titrosampler with accessories and printer

Ordering Information

2.862.1010	862 Food/Beverage Compact Titrosampler
2.862.1110	862 Food/Beverage Compact Titrosampler with printer
2.862.2010	862 Salt Compact Titrosampler
2.862.2110	862 Salt Compact Titrosampler with printer

Robotic Analyzer packages

Robotic Chloride Analyzer (2.855.1010)

The complete package for the determination of chloride contains all the components for a fully automatic chloride titration in the smallest possible space in a minimum of time. Instruments, accessories, software and application know-how – simply everything is included.



Robotic Acid-Base Analyzer (2.855.1020)

The complete package for the determination of acids and/or bases contains all the components for a fully automatic acid-base titration in the smallest possible space in a minimum of time. Instruments, accessories, software and application know-how – simply everything is included.



Robotic TAN/TBN Analyzer (2.855.2010)

The complete package for the determination of TAN and/or TBN contains all the components for a fully automatic TAN/TBN titration in the smallest possible space in a minimum of time. Instruments, accessories, software and application know-how – simply everything is included.



Robotic Fluoride Analyzer (2.855.2020)

The complete package for the determination of fluoride contains all the components for a fully automatic fluoride titration in the smallest possible space in a minimum of time. Instruments, accessories, software and application know-how – simply everything is included.




Robotic Transfer Analyzer (2.855.3020)

The complete package for the determination of acid and base contents in very high numbers of samples contains all the components for a fully automatic acid/base titration in the smallest possible space in a minimum of time. Instruments, accessories, software and application know-how – simply everything is included.



Sample preparation systems

An overview of sample preparation

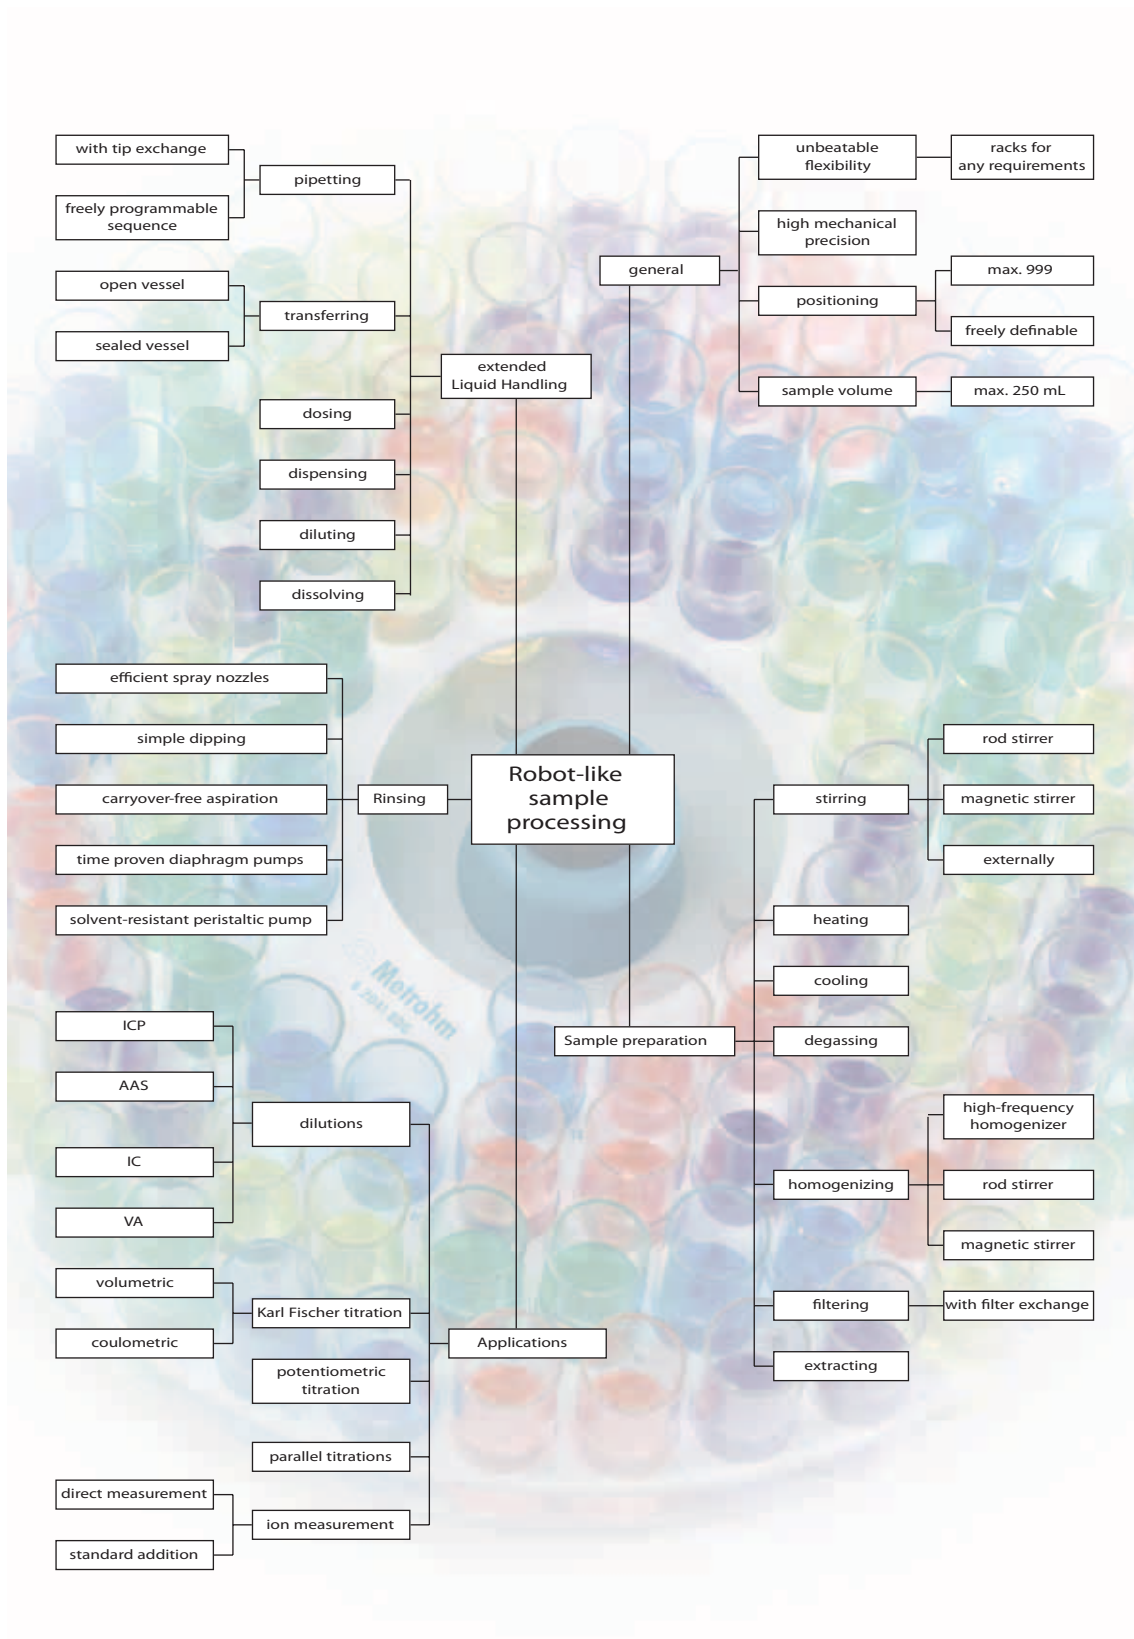

Robotic Soliprep

The Metrohm automation program has long offered you the opportunity of transferring your titration applications to a completely automated system. The Robotic Soliprep is a new version of the proven 815 Robotic USB Sample Processor that makes everyday routine work easier. The main area of utilization for the Robotic Soliprep systems is professional sample preparation. The Robotic Soliprep family is comprised of four packages that cover the different standard sample preparation steps. All Soliprep systems offer the possibility of homogenizing solid samples quickly and conveniently.

Up to 59 samples can be processed in a single run with the **Robotic Titration Soliprep**. The sample needs only be weighed into the beaker and placed on the sample rack. The reduction of the sample takes place subsequently with the Polytron 1300 D. After homogenization, the sample is titrated at the other workstation.

Up to 24 samples can be placed on the rack of the **Robotic Filtration Soliprep**. The reduction of the sample takes place with the Polytron 1300 D. During the following preparation steps, the Polytron aggregate is

cleaned in the external rinsing station. After the homogenization, an aliquot of the sample is aspirated and subsequently filtered through a commercially available syringe filter (Luer connector). The Dosino used for the sample transport doses the sample at uniform speed onto the filter, thus ensuring optimum filtration results. Needles and filters are replaced for each sample and disposed of safely in the collection container after use.

Up to 10 samples can be placed on the rack of the **Robotic Flexible Soliprep**. Further steps proceed as already described for the Robotic Filtration Soliprep. The filtrate can subsequently be pipetted, either directly or after additional dilution, in septum-sealed vials (11.6 mm). After completion of the series, the prepared samples can be easily removed from the sample rack in order to set the samples on the analyzer (e.g., IC or HPLC).

Up to 24 samples can be placed on the **Robotic Flexible Soliprep for LC**. After homogenization, an aliquot of the sample is aspirated using a metal-free plastic needle and subsequently transported through a commercially available syringe filter (Luer connector) and the Luer connector directly into the sample loop of the liquid chromatograph (LC).

The control of this preparation system takes place completely using the proven and flexible **tiamo**[™] titration software or the **MagIC Net** chromatography software that can also document the individual preparation steps for each sample in a database.



815 Robotic Filtration Soliprep

Ordering Information

2.815.1110	815 Robotic Titration Soliprep
2.815.2110	815 Robotic Flexible Soliprep
2.815.3110	815 Robotic Filtration Soliprep
2.815.4110	815 Robotic Soliprep for LC

Options

6.9012.000	Dispersing aggregate for Polytron, 125 mm
6.9012.010	Dispersing aggregate for Polytron, 157 mm

Automation peripheral devices

Membrane pumps

Liquids must frequently be pumped during titrations. The aspiration of the titrated-out sample solution is particularly convenient with automation. Following automatic run-through of the preprogrammed rinsing and aspiration cycles, the cleaned sample beakers and the electrodes that were used are available immediately for the next determination. The waste is transferred to canisters standing by for convenient disposal.

The **823 Membrane Pump** is a pump that can be used for many different applications. It was designed especially for operations and laboratory application and can be used for a broad spectrum of applications. It is suitable for pumping liquid media of any type and opens up a wide spectrum of applications with a flow rate of at least 450 mL/min.

The **843 Pump Station** (membrane) has two built-in membrane pumps. These can be controlled either via the interface either directly using remote signals or manually at the press of a button.

The two instruments are available in different versions that differ primarily with respect to the accessories supplied with them.



843 Pump Station Membrane

Ordering Information

2.823.0010	823 Membrane Pump Unit
2.823.0020	823 Membrane Pump Unit «aspirate»
2.823.0030	823 Membrane Pump Unit «rinse»
2.843.0020	843 Pump Station (membrane)
2.843.0030	843 Pump Station (membrane) - rinse/aspirate for Compact Sample Changer
2.843.0050	843 Pump Station (membrane) - rinse/aspirate for Sample Processors

Peristaltic pumps

Liquids must frequently be pumped during titrations. The aspiration of the titrated-out sample solution is particularly convenient with automation. Following automatic run-through of the preprogrammed rinsing and aspiration cycles, the cleaned sample beakers and the electrodes that were used are available immediately for the next determination. The waste is transferred to canisters standing by for convenient disposal. A membrane pump can no longer be used with liquids that contain solids such as silver chloride precipitates.

A peristaltic pump such as the **772 Pump Unit** is to be preferred in such cases. Here, the user has the opportunity of using pump tubing made of a wide variety of materials and thus to adjust the resistance of the tubing to the medium to be pumped in optimal fashion. One tubing for aqueous applications and one for organic solvents are shipped as standard equipment along with the Pump Unit.

The **843 Pump Station** (peristaltic) has two built-in peristaltic pumps. These can be controlled either via the interface either directly using remote signals or manually at the press of a button. The two instruments are available in various versions that differ primarily with respect to the accessories supplied with them.



843 Pump Station Peristaltic

Ordering Information

2.843.0120	843 Pump Station (peristaltic)
2.843.0130	843 Pump Station (peristaltic) - rinse/ aspirate for Compact Sample Changer
2.843.0150	843 Pump Station (peristaltic) - rinse/ aspirate for Sample Processors
2.772.0110	772 Pump Unit
2.772.0120	772 Pump Unit – aspirate
2.772.0130	772 Pump Unit – rinse

849 Level Control

Additional equipment for Sample Processors for monitoring the filling level of rinsing or waste canisters via Remote. It prevents pumps from running dry and/or canisters from overflowing and is suitable for use with aqueous solutions, solvents and suspensions.

The 849 Level Control can register both high liquid levels (e.g. warning that a waste container is about to overflow) and low liquid levels (e.g. storage container is about to run dry). Thanks to the conductivity measurement technique the level sensors can be used in different media.

The sensor signal is registered by the Level Control and transmitted as a signal level to a remote connection of an automated system. This means that the 849 Level Control can be used in all Metrohm systems in which it is possible to scan remote lines.



849 Level Control with canister

Ordering Information

2.849.0010	849 Level Control
2.849.0020	849 Level Control metal-free (for canisters)
2.849.0030	849 Level Control MF (for bottles)

731 Relay Box

- Two 115/230 V AC outputs
- Two DC outputs
- One standard cable is sufficient for communication with all Metrohm instruments

Additional device for controlling up to four external devices such as pumps or valves with mains connection or direct current consumers via TTL signals, including connection cable for devices with a 25-pin «remote» interface.

Automated systems require the switching of heaters, pumps, valves, thermostats or other external devices. This requires the use of relays to switch mains or low-voltage supplies on and off as necessary. The switching should take place via remote lines from a Titrino, Titrando, sample changer or other Metrohm instrument. The Relay Box meets all these requirements on a very small footprint.

The Relay Box provides four voltage outputs. Two 115/230 V AC outputs are used for switching the mains voltage. The maximum power delivery per output is 1'150 W, so that the instrument can also be used for providing power to high-consumption devices such as heating baths or thermostats.

In addition, the Relay Box has two DC outputs, whose voltages can be set to 5, 10, 18 or 24V.

Various Metrohm devices can be connected to the Relay Box via their remote interfaces. Regardless of the type of device, a single standard cable is all that is required for communication. The Relay Box scans the 14 input lines and switches the assigned voltage outputs accordingly.



731 Relay Box

Ordering Information

2.731.0010 731 Relay Box

786 Swing Head

Additional equipment for the Robotic Sample Processor XL for transferring / pipetting from smaller sample vessels into larger titration vessels on a rack or into an external titration cell that can be attached to the side of the work station.

With a Swing Head, the number of samples and their sizes can be varied within a wide range. This increased flexibility results from the considerable extension of the range of positions that can be reached on the Sample Processor. The Swing Head works with highest accuracy: it moves pipette / transfer tips from one position to the next, millimetre by millimetre. Even sample transfer into an external titration cell is carried out fully automatically, thus greatly increasing the flexibility of the Sample Processor. While the transferred sample is analyzed in the cell, the next sample is already being prepared; this means an additional gain in time. In addition, the Swing Head can also be equipped with Robotic Arms that can take up and eject tools or serve as a holder for a homogenizer for comminuting tablets.



Reinforced 786 Swing Head

Ordering Information

2.786.0010	786 Swing Head with transfer head left
2.786.0020	786 Swing Head with transfer head right
2.786.0030	786 Swing Head with titration swing arm, left- or right-swinging
2.786.0040	786 Swing Head
2.786.0240	786 Swing Head, right-swinging, reinforced

Stirrer

741 Magnetic Stirrer (2.741.0010)

Magnetic stirrer for sample changers.

The magnetic stirrer is located beneath the sample rack.



802 Stirrer (2.802.0020)

Rod stirrer for sample changer and Sample Processor.

With 6.1909.020 Propeller stirrer 104 mm and fixed cable.





Polarography, voltammetry and CVS



Polarography, voltammetry and CVS

Trace analysis with voltammetry	90
Determination of total metal and metal species	90
797 VA Computrace for trace analysis	91
797 VA Computrace with automatic standard addition for trace analysis	92
797 VA Computrace fully automated for trace analysis	93
Electrode kits for trace analysis	94
Sample preparation for trace analysis	95
909 UV Digester (230 V)	95
CVS – Cyclic Voltammetric Stripping	96
Introduction CVS	96
894 Professional CVS manual	97
894 Professional CVS semiautomated	98
894 Professional CVS fully automated for small sample series	99
894 Professional CVS fully and flexibly automated for large sample series	100
Electrode kits for CVS	101
Portable potentiostat	103
910 PSTAT mini	103

Trace analysis with voltammetry

Determination of total metal and metal species

Voltammetry instruments from Metrohm are modest in terms of servicing requirements, procurement price and dimensions, but nonetheless great in their detection capabilities.

Traces of toxic heavy metals can be analyzed in extremely low concentrations without great effort. The detection limits are to be found without exception in the ppt range, which means that the necessary sensitivity can be achieved in all cases. Voltammetry is one of the few methods in existence for the speciation of analytes.

Metal analyses can be carried out with equivalent or better sensitivity, at a fraction of the procurement price of an AAS or ICP instrument. An additional plus for voltammetry are the low costs of ownership. Except for small quantities of reagents, only tiny amounts of high-purity nitrogen are required. No expensive flammable gases, no conversion of the laboratory with special gas supply and flue gas outlets, no expensive lamps and no time-consuming calibration of the analysis system.

Applications that convince

Analysis of traces of metals

In addition to the determination of total concentrations, as is usual with spectroscopic methods, with voltammetry it is also possible to specify between the different oxidation stages of metal ions or the biological availability of heavy metals. A distinction can be made between free and bound metal ions. This makes voltammetry an indispensable element of environmental analysis. It is not possible for spectroscopy to yield comparable statements except after tedious separation of the metal species. Thanks to its compact dimensions, the instrument can also be used in mobile laboratories.

Samples with high ion concentrations present no problem for voltammetry. Voltammetry is predestined for the analysis of:

- Water, waste water and sea water
- Foods
- Salts, pure chemicals
- Galvanic baths

Specific analysis of organics

It is not only metals that can be determined, but also various organic compounds. The technology is used in organic chemistry, e.g. for the analysis of contaminations, or in pharmaceutical chemistry for the determination of active ingredient concentrations.

Examples of interesting determinations:

- 4-carboxybenzaldehyde in terephthalic acid
- Free styrol in polystyrene
- Vitamins in juices, vitamin preparations

Determination of anions

Some anions can also be determined with voltammetry. Of particular interest is the analysis of the species cyanide, sulfide, nitrite, nitrate and iodide.-

Sb ^{III} / Sb ^V	200 ppt
As ^{III} / As ^V	100 ppt
Bi	500 ppt
Cd	50 ppt
Cr ^{III} / Cr ^{VI}	25 ppt
Co	50 ppt
Cu	50 ppt
Fe ^{II} / Fe ^{III}	50 ppt
Pb	50 ppt
Hg	100 ppt
Mo	50 ppt
Ni	50 ppt
Pt	0.1 ppt
Rh	0.1 ppt
Se ^{IV} / Se ^{VI}	300 ppt
Tl	50 ppt
W	200 ppt
U	25 ppt
Zn	50 ppt

1 ppt = part per trillion = 1 ng/kg

Typical detection limits in voltammetric trace analysis

797 VA Computrace for trace analysis

The 10 most important benefits

- Voltammetric trace analysis and additive determination in galvanics with a single instrument
- Maximum sensitivity thanks to the combination of the unique Multi-Mode Electrode pro with the installed potentiostat
- Automation with the 863 Compact VA Autosampler or the 838 Advanced VA Sample Processor
- Archiving of the data in the Autodatabase program with report generator
- More than 220 important analysis methods are included in the scope of delivery
- Output of the result in an unlimited number of formats
- Unique EXPLORATORY mode, specially designed for education at schools and universities
- Metrohm monographs „Introduction to Polarography and Voltammetry“ and „Practical Voltammetry“
- Built-in quality assurance with GLP mode, access rights for each user and automatic electrode test
- Simple operation using the clearly organized user interface oriented to the Windows operating concept
- Connection to the USB port of the PC

The 797 VA Computrace is a modern voltammetric measuring stand that is connected to a PC via a USB port. The computer software provided controls the measurement, records the measured data and evaluates it. Operation is most straightforward due to the well-laid-out structure of the program. The integrated potentiostat with galvanostat guarantees the highest sensitivity with reduced noise.

Voltammetry system for trace analysis and education. Complete accessories with VA Computrace software and all electrodes for a complete measurement system: Multi-Mode Electrode pro (MME pro), Ag/AgCl reference electrode and Pt auxiliary electrode.

797 VA Computrace – Manual or automated

The 797 VA Computrace is a completely functional analysis system for meeting the highest expectations in terms of accuracy and sensitivity. All solutions are added manually. The various extension options, e.g., Dosinos or the additions of auxiliary and standard solutions, sample changer and automatic rinsing provide greater convenience.



797 VA Computrace

Ordering Information

2.797.0010 797 VA Computrace for trace analysis

797 VA Computrace with automatic standard addition for trace analysis

Easy to operate, partially automated analysis system for voltammetric trace analysis and education, comprised of 797 VA Computrace with two 800 Dosinos for the automatic addition of auxiliary solutions. The computer software provided controls the measurement, records the measured data and evaluates it. Operation is most straightforward due to the well-laid-out structure of the program. The integrated potentiostat with galvanostat guarantees the highest sensitivity with reduced noise.

Partially automated voltammetry system for inexpensive convenience

Two auxiliary solutions can be added automatically to the measuring vessel. Calibration in voltammetry is accomplished by means of standard addition or calibration curve and is carried out automatically by one of the 800 Dosinos. The second 800 Dosino adds the electrolytes or buffer automatically. The Dosinos are completely controlled by the 797 VA Computrace. One additional 800 Dosino can be connected directly, as can four additional ones by using an 846 Dosing Interface. A maximum of seven 800 Dosinos can thus be used.

The sample is handled manually. The sample is added in the measuring vessel by using a pipette and the analysis is started. This system is intended for users who value elegant and convenient operation at an attractive price without having to use a sample changer.

Complete accessories in the scope of delivery with VA Computrace software and all electrodes for a complete measurement system: Multi-Mode Electrode pro (MME pro), Ag/AgCl reference electrode and Pt auxiliary electrode.



MVA-02

Ordering Information

MVA-02 797 VA Computrace with automatic standard addition for trace analysis

797 VA Computrace fully automated for trace analysis

Fully automated analysis system for voltammetric trace analysis and education, comprised of 797 VA Computrace with 863 Compact VA Autosampler and two 800 Dosinos for the automatic addition of auxiliary solutions. The computer software provided controls the measurement, records the measured data and evaluates it. Operation is most straightforward due to the well-laid-out structure of the program. The integrated potentiostat with galvanostat guarantees the highest sensitivity with reduced noise.

Fully automated voltammetry system

Up to 18 samples can be investigated automatically, precisely and reproducibly. The software of the 797 VA Computrace controls the complete analysis sequence. The samples are placed on the sample rack of the 863 Compact VA Autosampler, and the rest takes place automatically: the transfer of the samples into the measuring vessel with the built-in peristaltic pump, the voltammetric determination with the automatic addition of all of the auxiliary solutions by using two 800 Dosinos and the automatic rinsing with the 843 Pump Station. The reproducible and efficient rinse minimizes carry-overs and thus

enhances the accuracy of the determinations. In order to increase the number of auxiliary solutions, one additional 800 Dosino can be connected directly, as can four additional ones by using an 846 Dosing Interface. A maximum of seven 800 Dosinos can thus be used.

This system is the optimum solution for the automatic analysis of small sample series that must be analyzed for one or two analytes in a single analysis run.

Complete accessories in the scope of delivery with VA Computrace software and all electrodes for a complete measurement system: Multi-Mode Electrode pro (MME pro), Ag/AgCl reference electrode and Pt auxiliary electrode.



MVA-03

Ordering Information

MVA-03 797 VA Computrace fully automated for trace analysis

Polarography, voltammetry and CVS

Electrode kits for trace analysis

MVA-Hg, equipment for mercury determination (6.5327.000)

Complete set of accessories for the determination of mercury as per Application Bulletin 96. Contains rotating gold working electrode, reference electrode, glassy-carbon auxiliary electrode and other accessories.

scTRACE Gold equipment (6.5340.000)

Complete accessories kit for the determination of arsenic with the scTRACE Gold as described in Application Bulletin 416. Contains electrode holder, scTRACE Gold (4 pieces), measuring vessel, stirrer and additional accessories.



Sample preparation for trace analysis

909 UV Digester (230 V)

- Control unit and wet end in a single housing
- Digital input of digestion temperature and digestion time
- Microprocessor-controlled regulation of digestion temperature and digestion time
- Air cooling
- Digestion of up to 12 samples simultaneously
- Short digestion times
- Largely blank value-free, as only very small amounts of reagents are required
- Also suitable for elements that form highly volatile compounds, e.g., mercury, arsenic and selenium

Digestion instrument for UV photolysis of water samples with low to medium organic load. For sample preparation in trace element determination by means of voltammetry, ion chromatography and spectroscopy (AAS, ICP). Integrated instrument with operating unit and wet end. With air cooling and automatic control of digestion temperature and time. For 12 samples with a maximum of 12 mL sample volume each. Instrument for 220 - 240 V and 50 - 60 Hz.

Digestion is indispensable for the reliable determination of traces and ultratraces of metals in natural samples, as organic sample components are generally disruptive to analysis. The 909 UV Digester was designed for the digestion of suspended particle-free water samples containing low to medium contents of organic material, e.g., natural surface waters. As a result of its low heavy metal content, contaminations can very easily lead to disruptions during determination. Liquid biological samples such as urine or some foodstuffs such as fruit juices and alcoholic beverages can however also be digested with a modified procedure. A great advantage of the UV digestion is that only small amounts of digestion reagents need to be used and therefore the blank values can be kept low.

12 samples can be radiated simultaneously in the 909 UV Digester.



909 UV Digester

Ordering Information

2.909.0014 909 UV Digester (230 V)

CVS – Cyclic Voltammetric Stripping

Introduction CVS

Cyclic Voltammetric Stripping Analysis (CVS) and *Cyclic Pulse Voltammetric Stripping Analysis (CPVS)* are methods widely used in the electroplating industry for the determination of organic additives in electroplating baths. A robust, inexpensive rotating disk electrode of simple construction made of platinum is installed in the VA stand for these analyses in place of the Multi-Mode electrode that is otherwise used. This method is an indispensable part of production control for many types of technical coatings and particularly in the manufacturing of printed circuit boards for electronic equipment. The most important fields of application are acidic copper baths and tin-lead baths. Quantitative determination of the additives takes place indirectly via their influence on the plating of the main component of the electroplating bath. As the measurement utilizes a procedure that corresponds to the production process, the activity of the additives and thus their effectiveness in the electroplating process is measured directly.

The quantification of the various types of additives requires special calibration techniques, all of which are available in Metrohm CVS systems. The so-called brighteners are determined with the aid of the *Linear*

Approximation Technique (LAT) or the *Modified Linear Approximation Technique (MLAT)*. *Dilution Titration (DT)* is used for the determination of the suppressors while levelers are determined via *Response Curve (RC)*.

The concentrations of the additives can be determined exactly with CVS or CPVS. The effective concentration of the respective additive in the bath sample is displayed and printed out directly in mL of additive per L of bath. Topping-up to achieve nominal concentration thus can be carried out very precisely as a result. This guarantees a continuous, malfunction-free production process. The accuracy of the analysis results in particular have led to the general acceptance of the method in the electroplating industry.

Other methods, e.g., the classical Hull cell method, do not allow the concentration to be determined, but only provide an assessment of the quality of the deposited metal layer.

One of the pre-installed methods is loaded to perform the determination. The analysis can be started once a few parameters have been adjusted. Pre-finished methods that have been formulated in our Applications Laboratory for the most important bath types of leading manufacturers are supplied along with the instrument.



894 Professional CVS manual

The most important benefits

- Compact instrument with small installation area
- Measuring head that can be replaced with a single hand movement
- Built-in certified calibrator for automatic instrument adjustment before each measurement
- Flexible Liquid Handling with 800 Dosinos
- Flexible automation options with 858 Professional Sample Processor, 919 IC Autosampler plus and 843 Pump Station
- Connection to the USB port of the PC

894 Professional CVS manual is the introductory instrument for the high-end determinations of organic additives in electroplating baths with „Cyclic Voltammetric Stripping“ (CVS). The proven Metrohm electrode technique in combination with a completely newly designed potentiostat/galvanostat and the extremely high-performance **viva** software opens up new perspectives in CVS. The replaceable measuring head enables rapid changes between various applications with different electrodes. The potentiostat with certified calibrator readjusts itself automatically before each measurement and guarantees a maximum in precision.



894 Professional CVS manual

The **viva** software is required for control, data recording and evaluation.

The 894 Professional CVS manual is supplied with extensive accessories and measuring head for rotating disk electrodes. Electrode set and **viva** license are to be ordered separately.

Manual system with versatile extension options

With the appropriate electrode set, the 894 Professional CVS manual is a completely functional analysis system for meeting the highest expectations in terms of accuracy and sensitivity. The measurement system offers maximum flexibility through modular extension options and the practically unlimited configurability available with the **viva** software.

viva

The Professional CVS system is controlled with **viva**. The new software for CVS offers previously unachieved flexibility with respect to method adjustment and automation and thus sets new standards in the determination of organic additives with CVS. **viva** is available in a single-user version or as a network option for one client-server installation.

Ordering Information

2.894.0210 894 Professional CVS manual

894 Professional CVS semiautomated

The most important benefits

- Compact instrument with small installation area
- Two 800 Dosinos for the automatic addition of auxiliary solutions
- Liquid Handling can be extended without limit with additional 800 Dosinos
- Measuring head that can be replaced with a single hand movement
- Built-in certified calibrator for automatic instrument adjustment before each measurement
- Flexible automation options with 858 Professional Sample Processor, 919 IC Autosampler plus and 843 Pump Station
- Connection to the USB port of the PC

894 Professional CVS semiautomated is a convenient high-end routine analyzer for determinations of organic additives in electroplating baths with „Cyclic Voltammetric Stripping“ (CVS). The proven Metrohm electrode technique in combination with a completely newly designed potentiostat/galvanostat and the extremely high-performance **viva** software opens up new perspectives in CVS. The replaceable measuring head enables rapid changes

between various applications with different electrodes. The potentiostat with certified calibrator readjusts itself automatically before each measurement and guarantees a maximum in precision.

Two 800 Dosinos (supplied) permit the automatic addition of auxiliary solutions during the determination, e.g., VMS, standard solutions or samples for the Dilution Titration technique (DT).

The **viva** software is required for control, data recording and evaluation.

The 894 Professional CVS semiautomated is supplied with extensive accessories and measuring head for rotating disk electrodes. Electrode set and **viva** license are to be ordered separately.

Convenient routine measurements

With the appropriate electrode set, the 894 Professional CVS semiautomated enables the determination of suppressors with Dilution Titration (DT). All solutions are added automatically during the determination by the two supplied 800 Dosinos, e.g., VMS, standard solutions or samples for the Dilution Titration technique (DT). The determination proceeds automatically, from the preparation of the sample to the calculation of the final result. The performance capability can be further increased through modular extension options and the practically unlimited configurability available with the **viva** software.

viva

The Professional CVS system is controlled with **viva**. The new software for CVS offers previously unachieved flexibility with respect to method adjustment and automation and thus sets new standards in the determination of organic additives with CVS. **viva** is available in a single-user version or as a network option for one client-server installation.



894 Professional CVS semiautomated with 800 Dosino

Ordering Information

2.894.1210 894 Professional CVS semiautomated

894 Professional CVS fully automated for small sample series

Automated analysis system for the determination of organic additives in electroplating baths using the CVS technique („Cyclic Voltammetric Stripping“). Comprised of 894 Professional CVS, 919 IC Autosampler plus, four 800 Dosinos, 843 Pump Station, measuring head for rotating disk electrodes and extensive accessories. For small sample series of up to 14 samples.

The **viva** software is required for control, data recording and evaluation. PC, electrode set and **viva** license are to be ordered separately.

Fully automated analysis system for the determination of organic additives with CVS in routine laboratory work

MVA-20 is the version in our top system for fully automated additive determination in electroplating baths with CVS (Cyclic Voltammetric Stripping) for small sample series. Up to 27 samples can be investigated with respect to suppressor content with the 919 IC Autosampler plus. Up to 14 samples can be analyzed automatically during brightener determination. The possibility of recalibrating methods during a sample series guarantees the highest

of accuracy. And different methods can be combined in a single measurement sequence.

The system is based on the 894 Professional CVS with four 800 Dosinos for the automatic addition of auxiliary solutions. VMS and the electroplating bath sample are added by using 800 Dosinos in cases of suppressor determination. For the determination of brighteners, the intercept solution and brightener standard solution are added by 800 Dosino dosing systems; the peristaltic pump of the 919 IC Autosampler plus is used for transferring the sample automatically from the sample vessel on the sample rack into the measuring vessel on the 894 Professional CVS. The attached 843 Pump Station empties and rinses the measuring vessel automatically after each sample.

viva

The Professional CVS system is controlled with **viva**. The new software for CVS offers previously unachieved flexibility with respect to method adjustment and automation and thus sets new standards in the determination of organic additives with CVS. **viva** is available in a single-user version or as a network option for one client-server installation.



MVA-20

Ordering Information

MVA-20 894 Professional CVS fully automated for small sample series

Polarography, voltammetry and CVS

894 Professional CVS fully and flexibly automated for large sample series

Automated analysis system for high-performance, flexible determination of organic additives in electroplating baths using the CVS technique („Cyclic Voltammetric Stripping“). Comprised of 894 Professional CVS, 858 Professional Sample Processor, four 800 Dosinos, 843 Pump Station, measuring head for rotating disk electrodes and extensive accessories. For sample series of up to 56 samples.

The **viva** software is required for control, data recording and evaluation. PC, electrode set and **viva** license are to be ordered separately.

Fully automated analysis system for the determination of organic additives with CVS in routine laboratory work

MVA-21 is the version in our top system for fully automated additive determination in electroplating baths with CVS (Cyclic Voltammetric Stripping) for large sample series. Up to 56 samples can be investigated with respect to suppressor content with the 858 Professional Sample Processor. Up to 28 samples can also be analyzed automatically during brightener determination. The possibility

of recalibrating methods during a sample series guarantees the highest of accuracy. And different methods can be combined in a single measurement sequence.

The system is based on the 894 Professional CVS with four 800 Dosinos for the automatic addition of auxiliary solutions. VMS and the electroplating bath sample are added by using 800 Dosinos in cases of suppressor determination. For the determination of brighteners, the intercept solution and brightener standard solution are added by 800 Dosino dosing systems; the peristaltic pump of the 858 Professional Sample Processor is used for transferring the sample automatically from the sample vessel on the sample rack into the measuring vessel on the 894 Professional CVS. The attached 843 Pump Station empties and rinses the measuring vessel automatically after each sample.

viva

The Professional CVS system is controlled with **viva**. The new software for CVS offers previously unachieved flexibility with respect to method adjustment and automation and thus sets new standards in the determination of organic additives with CVS. **viva** is available in a single-user version or as a network option for one client-server installation.



MVA-21

Ordering Information

MVA-21 894 Professional CVS fully and flexibly automated for large sample series

Electrode kits for CVS

CVS electrode equipment with 1 mm platinum electrode for Professional CVS instruments (6.5339.000)

Complete electrode set for the determination of organic additives in electroplating baths with CVS (Cyclic Voltammetric Stripping). Contains rotating platinum working electrode (electrode diameter: 1 mm), reference electrode, platinum auxiliary electrode and electrolyte solutions.

CVS electrode equipment with 2 mm platinum electrode for Professional CVS instruments (6.5339.010)

Complete electrode set for the determination of organic additives in electroplating baths with CVS (Cyclic Voltammetric Stripping). Contains rotating platinum working electrode (electrode diameter: 2 mm), reference electrode, platinum auxiliary electrode and electrolyte solutions.

CVS electrode equipment with 3 mm platinum electrode for Professional CVS instruments (6.5339.020)

Complete electrode set for the determination of organic additives in electroplating baths with CVS (Cyclic Voltammetric Stripping). Contains rotating platinum working electrode (electrode diameter: 3 mm), reference electrode, platinum auxiliary electrode and electrolyte solutions.



viva – Software for CVS

Modern, user-friendly software for the performance of CVS determinations. Thanks to its easy operation and maximum flexibility, **viva** enables individual and problem-oriented method programming for CVS measuring technology for the first time.

The „Workplace“ program part is the cockpit of **viva**. Here all of the information necessary for the determination is visible at a glance. It goes without saying that the „Workplace“ can be individually configured so that only the data relevant to the user is displayed. The method used and the associated evaluation parameters are logically structured and clearly displayed in the method window. The measured voltammograms and the associated calibration curve are displayed in the curve window.

viva is the first and only software for CVS that enables individual, problem-oriented method programming with the aid of a graphical method editor. Numerous templates simplify method development. The intelligence functions of **viva** make it possible to have the run of the method be made dependent on results of the current measurement that have already been calculated. Thus,


for example, standard addition volumes can be calculated autonomously.

All determinations are stored in a database for convenient data management where they can be viewed along with all of the determination, method and instrument parameters.

The most important features at a glance:

- Freely configurable determination overview
- High-performance sort, search and filter functions that are simple to operate
- Recalculation and recalibration functions
- Report generator for customized structuring of the analysis report
- Client-server version for the central storage of all methods and determinations on a single server. All measured data is thus available throughout the company
- Freely definable access permissions for each user

viva is available in the **viva** Full single-user version with 1 license for one computer. The alternative is the **viva** Multi client-server version with 3 licenses for three computers for company networks, which makes it possible to store all of the data on a central server. Separate licenses can be obtained for additional computers.

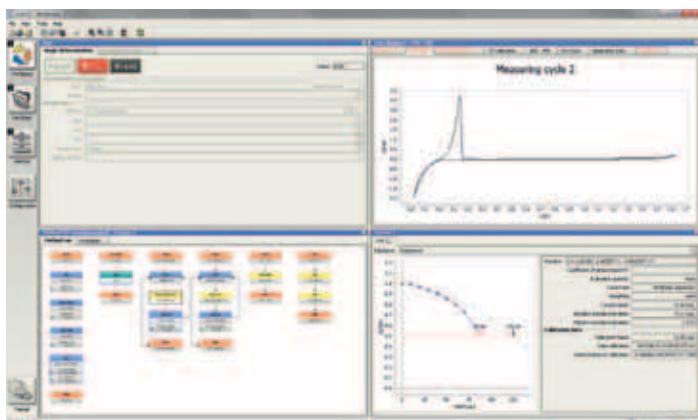

viva workplace

Ordering Information

6.6065.102 viva 1.0 Full CD: 1 license

6.6065.103 viva 1.0 Multi CD: 3 licenses

Portable potentiostat

910 PSTAT mini

- Small and compact
- Mobile
- Inexpensive
- All of the important electrochemical measurement techniques
- Maintenance-free disposable sensors
- Power supply via USB
- Simple, intuitive PSTAT software
- Monograph „Electrochemistry – A workbook for 910 PSTAT mini“

The ideal introductory instrument for electrochemistry

910 PSTAT mini is a small and compact, PC-controlled potentiostat with USB connector for training purposes as well as simple applications in research and development. The PSTAT software provided is easy and intuitive to operate and covers the most important electrochemical measuring techniques. Included in the scope of delivery are inexpensive disposable thick film sensors that can be utilized directly, without preparation and conditioning.

The 910 PSTAT mini is supplied with extensive accessories in a transport case.

The most important applications

- Training in electrochemistry (student internships, demonstration experiments)
- Electrochemical research and development (sensor development, reversibility of electrochemical reactions, reaction kinetics)

PSTAT software

As a result of its intuitive operability, PSTAT software is particularly suitable for training in electrochemistry. Measurement is of the essence. That is why the software includes only those functions that are really important for measurement, i.e. measuring parameters, curves and manual signal evaluation. All of the fundamental electrochemical measurement techniques are available: Cyclic Voltammetry (CV) for investigating the mechanism and kinetics of electrode reactions or for characterizing modified sensors; Differential Pulse Voltammetry (DP) and Square Wave Voltammetry (SWV) for quantitative determination of electrochemically active substances such as mercury, organic substances or cadmium and lead after modification. Chronoamperometric Detection (AD) for demonstrating the functional principle of an amperometric biosensor such as a glucose sensor.

Screen-printed electrodes (SPE)

Inexpensive disposable thick film electrodes make electrochemistry easy. The electrode is inserted into the holder and measurement can begin without further preparation. Each sensor contains the 3 required electrodes: the working electrode, made of carbon, gold or platinum, a silver reference electrode and a carbon auxiliary electrode on a ceramic holder.

Monograph „Electrochemistry – A workbook for 910 PSTAT mini“

The monograph provides an easy introduction to the field of electrochemistry. The book in its handy format includes experiments that describe fundamental phenomena of electrochemical analytics. These experiments can be readily carried out with the 910 PSTAT mini and the electrodes supplied.



910 PSTAT mini

Ordering Information

2.910.0010 910 PSTAT mini



Stability measuring instruments



Stability measuring instruments

Oxidation stability of fats and oils 108

892 Professional Rancimat 108

Oxidation stability of biodiesel and biodiesel blends 109

893 Professional Biodiesel Rancimat 109

Thermostability of PVC 110

895 Professional PVC Thermomat 110

Software for stability measuring instruments 111

StabNet 111

Oxidation stability of fats and oils

892 Professional Rancimat

- Control of all the instrument functions from the computer
- Individual start of each measuring position directly on the instrument
- Overview of the status of all measuring positions on the instrument display
- Highest reliability and simple operation through unique accessories
- Inexpensive disposable glass components
- Robust conductivity measuring cell with electrical connections integrated in the lid
- 2 heating blocks with 8 measuring positions per instrument. Up to 4 instruments can be connected to a PC
- Expanded gas flow range: 1 - 25 L/h
- USB connector
- Compact dimensions and low weight

Analysis system for the simple and safe determination of the oxidation stability of natural fats and oils with the well-established Rancimat method. All accessories necessary for carrying out determinations are included in the scope of delivery. The StabNet software is required for instrument control, data recording and evaluation and for data storage.



892 Professional Rancimat

Oxidation stability of fats and oils in the food industry

The Rancimat method is used as a default parameter in the food industry for quality control during the manufacture of fats and oils, or for incoming goods checks in processing industries. In addition to vegetable oils and fats, it is also possible to check animal fats such as lard, tallow or fish oil. It is also possible, with the help of the 892 Professional Rancimat, to characterize the effectiveness of antioxidants that are added to foods in order to slow down oxidative decomposition.

Standards

- AOCS Cd 12b-92 (AOCS - American Oil Chemists' Society): Sampling and analysis of commercial fats and oils: Oil Stability Index
- ISO 6886: Animal and vegetable fats and oils - Determination of oxidative stability (accelerated oxidation test)
- 2.4.28.2-93: Fat stability test on Autoxidation. CDM, Japan

Oxidation stability of fat-containing foods

The 892 Professional Rancimat can also be used for the determination of the oxidation stability of fat-containing foods. Examples:

- Instant noodle dishes
- Nuts, almonds
- Cookies, biscuits
- Potato chips and similar snacks

Oxidation stability of cosmetics

In addition to foods, the oxidation stability of aliphatic cosmetics or of cosmetics additives can also be determined with the help of the 892 Professional Rancimat.

Ordering Information

2.892.0010 892 Professional Rancimat

Oxidation stability of biodiesel and biodiesel blends

893 Professional Biodiesel Rancimat

- Control of all the instrument functions from the computer
- Individual start of each measuring position directly on the instrument
- Overview of the status of all measuring positions on the instrument display
- Highest reliability and simple operation through unique accessories
- Inexpensive disposable glass components
- Robust conductivity measuring cell with electrical connections integrated in the lid
- 2 heating blocks with 8 measuring positions per instrument. Up to 4 instruments can be connected to a computer
- Expanded gas flow range: 1 - 25 L/h
- USB connector
- Compact dimensions and low weight

Analysis system for simple and safe determination of the oxidation stability of biodiesel (fatty acid methyl esters, FAME) and biodiesel blends in accordance with the standards EN 14112, EN 15751 and EN 16568. All accessories necessary for carrying out determinations are included in the scope of delivery. The StabNet software is required for instrument control, data recording and evaluation and for data storage.

Oxidation stability of biodiesel (fatty acid methyl esters, FAME), biodiesel blends and diesel

Biodiesel has relatively little storage stability, as it (like natural fats and oils) is slowly oxidized by atmospheric oxygen. The substances that arise thereby could lead to damage in the motor. It is for this reason that oxidation stability is an important default parameter in a series of standards that define the minimum quality standards of biodiesel. This determination can be carried out simply and reliably with the 893 Professional Biodiesel Rancimat.

Standards

Testing requirements

- ASTM D 6751 (ASTM - American Society for Testing and Materials) „Standard specification for biodiesel fuel blend stock (B100) for middle distillate fuels“
- ASTM D 7467 „Standard Specification for Diesel Fuel Oil, Biodiesel Blend (B6 to B20)“
- EN 14214 „Liquid petroleum products - Fatty acid methyl esters (FAME) for use in diesel engines and heating applications - Requirements and test methods“
- EN 590 „Automotive fuels - Diesel - Requirements and test methods“

Test methods

- EN 14112 „Fat and oil derivatives - Fatty acid methyl esters (FAME) - Determination of oxidation stability (accelerated oxidation test)“
- EN 15751 „Automotive fuels - Fatty acid methyl esters (FAME) fuel and blends with diesel fuel - Determination of oxidation stability by accelerated oxidation method“
- EN 16568 „Automotive fuels - Fatty acid methyl esters (FAME) fuel and blends with diesel fuel - Determination of oxidation stability by rapidly accelerated oxidation method at 120 °C“



893 Professional Biodiesel Rancimat

Ordering Information

2.893.0010 893 Professional Biodiesel Rancimat

Thermostability of PVC

895 Professional PVC Thermomat

- Control of all the instrument functions from the computer
- Individual start of each measuring position directly on the instrument
- Overview of the status of all measuring positions on the instrument display
- Highest reliability and simple operation through unique accessories
- Inexpensive disposable glass components
- Robust conductivity measuring cell with electrical connections integrated in the lid
- 2 heating blocks with 8 measuring positions per instrument. Up to 4 instruments can be connected to a computer
- Expanded gas flow range: 1 - 25 L/h
- USB connector
- Compact dimensions and low weight

Analysis system for the automatic determination of the thermostability of poly(vinyl chloride) (PVC) and related copolymers. All accessories necessary for carrying out determinations are included in the scope of delivery. The StabNet software is required for instrument control, data recording and evaluation and for data storage.

Thermostability of PVC

Chlorinated plastics based on poly(vinyl chloride) (PVC) decompose at higher temperatures with accompanying release of gaseous HCl. The thermostability of the PVC material is defined as the time until HCl is released and is determined by the measurement of a defined conductivity change in the measuring cell.

Standards

- DIN 53381-1 „Testing of plastics; determination of thermostability of polyvinyl chloride (PVC); dehydrochlorination methods“
- ISO 182-3 „Plastics - Determination of the tendency of compounds and products based on vinyl chloride homopolymers and copolymers to evolve hydrogen chloride and any other acidic products at elevated temperatures - Part 3: Conductometric method“



895 Professional PVC Thermomat

Ordering Information

2.895.0010 895 Professional PVC Thermomat

Software for stability measuring instruments

StabNet

Modern, user-friendly software for control and data handling of stability measuring instruments. The software permits checks, data acquisition, evaluation and monitoring, as well as report generation of stability measurements.

Graphical user interface for routine operations, extensive database programs, method development, system configuration, very flexible user administration, extensive data export functions, individually configurable report generator. StabNet fulfills the directives pursuant to FDA 21 CFR Part 11.


All determinations are stored in a database for convenient data management where they can be viewed along with all of the determination, method and instrument parameters.

The most important features at a glance:

- Clear and structurally well-organized user interface
- Database with flexible functions for filtering, sorting and statistics
- High transparency of results by storage of all determination, method and instrument parameter data and the history when measured data is reevaluated or recalculated

- High data security due to manipulation-proof database and automatic backup functions
- User administration with freely configurable access rights
- In compliance with all GLP and FDA requirements

StabNet is available in the StabNet Full single-user version with 1 license for a max. of 4 stability measuring instruments on one computer. The alternative is the StabNet Multi client-server version with 3 licenses for three computers for company networks, which makes it possible to store all of the data on a central server. Separate licenses can be obtained for additional computers.

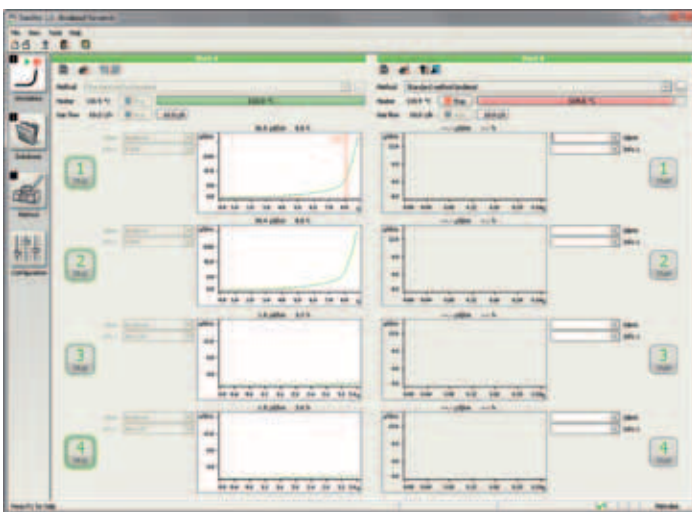

StabNet workplace

Ordering Information

- | | |
|------------|----------------------------------|
| 6.6068.102 | StabNet 1.0 Full CD: 1 license |
| 6.6068.103 | StabNet 1.0 Multi CD: 3 licenses |



Near-infrared spectroscopy



Near-infrared spectroscopy

Introduction to near-infrared spectroscopy	116
Overview of NIRS instruments	116
Metrohm NIRSystems	117
Laboratory and atline for solid samples	118
Introduction	118
NIRS DS2500 Analyzer	119
NIRS XDS – the all-rounder	120
Laboratory and atline for liquid samples	121
Introduction	121
NIRS XDS RapidLiquid Analyzer	122
Fiber Optics – the flexible ones	123
Process analyzers	124
Introduction	124
NIRS XDS Process Analyzers – SingleFiber	125
NIRS XDS Process Analyzers – MicroBundle	126
NIRS XDS Process Analyzer – DirectLight/ NonContact	127
NIRS Analyzer PRO	128

Introduction to near-infrared spectroscopy





Overview of NIRS instruments

Near-infrared spectroscopy (NIRS) is a versatile analysis procedure that has been applied successfully in the pharmaceutical and chemical industries for more than 25 years.

This simple, rapid (< 30 s measuring time) and non-destructive physical measurement method offers, for practically every sample matrix, an accurate and precise analysis of chemical and physical parameters comparable to reference methods. As an additional major benefit, near-infrared (NIR) analyses require no sample preparation or the use of hazardous chemicals, solvents or reagents.

The Metrohm NIR product range comprises not only the simple and intuitive NIR laboratory analyzers, but also robust, user-friendly NIR process analyzers.


- Dedicated systems
- Temperature controller up to 65 °C
- Optional temperature controller up to 200 °C
- ▲ Different fiber optic probes are available
- ▲ With transreflectance options



Sample type	Laboratory analyzer, atline analyzer								
	XDS Rapid ContentAnalyzer	XDS Rapid Content Solid Analyzer	XDS MultiVial Analyzer	XDS MasterLab Analyzer	XDS RapidLiquid Analyzer	XDS SmartProbe Analyzer	XDS Interactance OptiProbe Analyzer	XDS Transmission OptiProbe Analyzer	DS2500 Analyzer
									
Powders	●	●	●	●		●	●		●
Coarse solids/ granulates		●	●	●		●	●		●
Solids/film/paper	●	●	●	●					●
Tablets/capsules in reflection	●	●	●	●					
Tablets/capsules in transmission				●					
Opaque liquids	●	●	▲	▲		●	●		●
Pastes/creams	▲	▲	▲	▲		●	●		▲
Viscous liquids/gels	▲	▲	▲	▲	●	●	●	●	
Clear liquids	▲	▲	▲	▲	●	▲	▲	●	▲

Metrohm NIRSystems

Metrohm offers NIR applications for all process environments. Metrohm NIRSystems instruments can be installed in the laboratory, atline or directly into a process stream, dryer, extruder, or reactor. The measurement mode and location of the analyzer depend on the optical properties of the samples, the required analyte selectivity

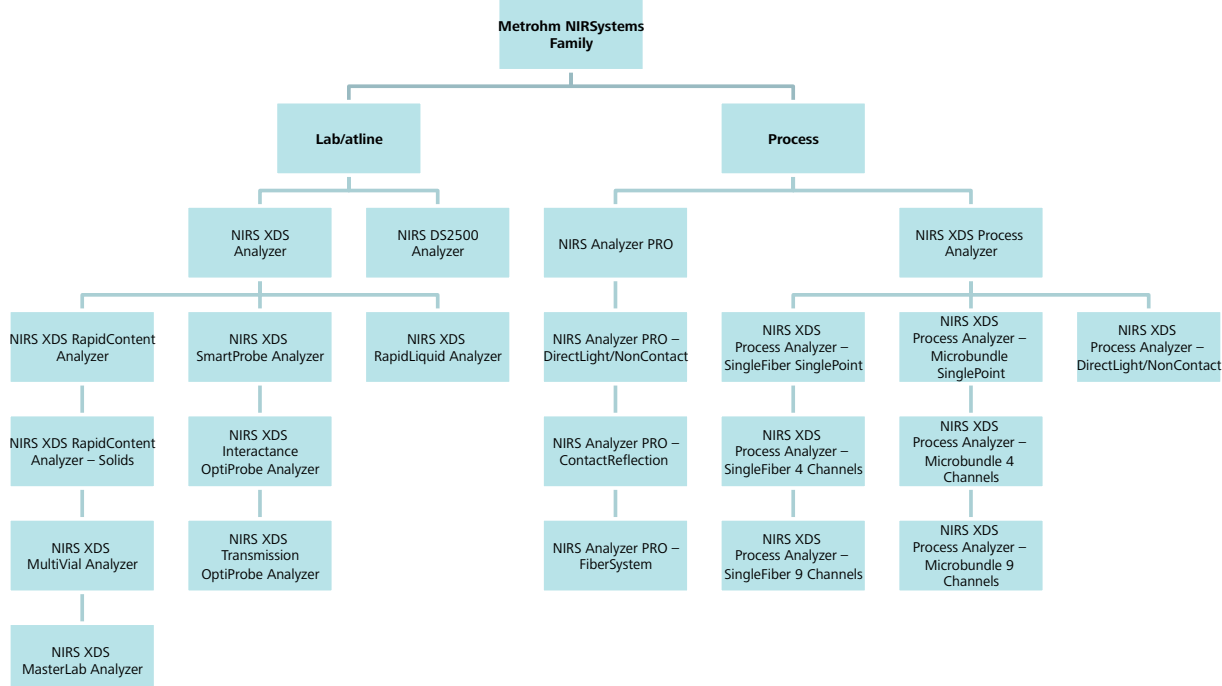and sensitivity, the duration of the process run and the monitoring and control requirements. Below is a short overview of Metrohm NIRSystems instruments. A suitable analyzer is available for every sample type and processing environment.



Sample type	Process analyzer					
	XDS Process Analyzer			NIRS Analyzer PRO		
	SingleFiber	MicroBundle	DirectLight	ContactReflection	Fiber	DirectLight
						
Powders		▲	●	●	▲	●
Coarse solids/ granulates		▲	●	●	▲	●
Solids/film/paper		▲	●	●	▲	●
Tablets/capsules in reflection						
Tablets/capsules in transmission						
Opaque liquids	▲	▲			▲	
Pastes/creams	▲	▲		●	▲	
Viscous liquids/gels	▲	▲			▲	
Clear liquids	▲	▲			▲	

Laboratory and atline for solid samples

Introduction

Metrohm NIRSystems laboratory analyzers with their patented monochromator can be operated in all laboratories: from quality control through research and development to plant laboratories. Modular sampling accessories allow for analyses of powders, granules, solids, slurries, gels, pastes, and turbid or clear liquids. Since NIR analyses are performed on unmodified samples, presenting the samples to the instrument is the most important aspect of NIR analysis. The modular design of Metrohm NIRSystems laboratory analyzers ensures that analyses are optimized for specific sample types.

The NIRS DS2500 Analyzer enables simple routine analyses in difficult environments and meets the standards of protection class IP65. True transmission and reflection measurements for solid dosage forms are carried out with the NIRS XDS MasterLab Analyzer.

The NIRS XDS RapidContent Analyzer performs reflectance analysis on materials in bags, vials, or sample beakers and transmittance analysis of liquids in beakers. The NIRS XDS RapidContent Analyzer with Solids Module provides large area sampling for nonhomogeneous powders, fibrous materials, flakes, and pellets.



NIRS DS2500 Analyzer

- Compact analyzer for reflectance measurements
- Maximum optical performance across the entire wavelength range (400 to 2,500 nm)
- Consistent results, even in harsh environments
- Network-capable via LAN (local) or direct PC connection
- New predispersive monochromator
- Several optional sampling accessories

Near-infrared analyses are becoming ever better. With the compact NIRS DS2500 Analyzer, near-infrared analysis has taken yet another step into the future of routine analysis. This dedicated analyzer offers exceptional accuracy across a broad wavelength range of 400 to 2,500 nm and is designed for use in the receiving area or atline in the nutraceutical industry.

Unmatched optical performance

The predispersive monochromator technology now being utilized in the NIRS DS2500 guarantees a high degree of versatility and stability across the entire spectral range from 400 to 2,500 nm. The NIRS DS2500 uses signal-noise ratio to perform, in less than one minute, high-precision analyses of parameters ranging

from very simple to sophisticated. With this high-performance instrument, you and your team can be sure that you are getting the highest level of quality control at all stages of production.

Specially developed for this purpose

The NIRS DS2500 Analyzer was created as a high-performance instrument for harsh production environments. Robust, easy-to-use and IP65 certified, it withstands humidity, dust, vibrations and temperature fluctuations. This solidity of its construction makes the NIRS DS2500 Analyzer suitable for atline use by anyone in any production plant. The NIRS DS2500 complies with pharma regulations and supports the workflows of the nutraceutical industry.



NIRS DS2500 Analyzer

Ordering Information

2.922.0010 NIRS DS2500 Analyzer

NIRS XDS – the all-rounder

The NIRS XDS family guarantees more rapid analyses and even more accurate results for quality control in the laboratory. With the NIRS XDS Analyzers, you can replace routine tests, reduce product hold time and virtually eliminate quarantine time.

The NIRS XDS Analyzer is part of a generation of dedicated NIR analysis instruments for rapid nondestructive measurements of solid chemical and pharmaceutical samples in addition to liquid samples. Special modules support optimum analysis performance. The presence of modules that can be exchanged during operation provides great flexibility.

Identification, qualitative and quantitative methods are easily created with the advanced, user-friendly, network-compatible Vision® software. Precise and accurate analysis is accomplished with the press of a key or click of the mouse.

Advantages

- Ease-of-use
- Robust and accurate
- Flexible
- Effortless method transferability



NIRS XDS RapidContent Analyzer

NIRS XDS RapidContent Analyzer/Solids

Composition or material identification testing is performed either in the laboratory or atline, on samples contained in their original vials, bags or bottles. The Solids Module extends analysis to virtually any solid form from fine powders to coarse granular materials, pellets, and flakes. An optional variable spot-size feature enables the sample illumination to be adjusted based on the physical properties of your samples.

NIRS XDS MultiVial Analyzer

The NIRS XDS MultiVial Analyzer supports acquisition of spectra in an unattended mode, freeing the operator to prepare other samples, analyze data, etc. The versatile sampling mechanism of the NIRS XDS MultiVial Analyzer offers a movable (X-Y) sampling platform, suitable for handling a tray of multiple vials. An integrated variable spot-size feature enables the sample illumination to be adjusted based on the diameter of the vials being used.

NIRS XDS MasterLab Analyzer

The NIRS XDS MasterLab Analyzer offers pharmaceutical manufacturers a rapid, reliable test method covering the full array of solid dosage forms: layered, coated or cored tablets, capsules, caplets, gel tabs and gel caps. The versatile sampling mechanism of the NIRS XDS MasterLab Analyzer offers an automated and unattended reflectance or transmission analysis of tablets or vials.

The optional sample cell for coarse granular substances extends analysis to nonhomogeneous solid forms ranging from fine powders to coarse granular materials, pellets and flakes by averaging over a large area.

Ordering Information

2.921.1110	NIRS XDS RapidContent Analyzer
2.921.1120	NIRS XDS RapidContent Analyzer – Solids
2.921.1210	NIRS XDS MultiVial Analyzer
2.921.1310	NIRS XDS MasterLab Analyzer

Laboratory and atline for liquid samples

Introduction

Metrohm NIRSystems offers dedicated NIR analyzers for the analysis of clear or viscous liquids that can be easily used in the quality control laboratory or at the production site. Temperature monitoring during measurement is very important with temperature-dependent aqueous and liquid samples. Because many oil-based samples are in solid form at room temperature, a heater and a temperature controller are required for increasing sample transparency for NIR spectral consistency.

It is for this reason that a temperature control feature is integrated into the Metrohm NIRS XDS RapidLiquid Analyzer for higher performance and accurate measurement. The NIRS XDS RapidLiquid Analyzer performs liquid analysis in controlled temperature environments at room temperature and up to 65 °C. The optional Vial Heater Module, with which the temperature can be heated up and controlled up to as high as 200 °C, is available for the NIRS XDS Transmission OptiProbe Analyzer.



NIRS XDS RapidLiquid Analyzer

- NIR XDS technology guarantees simple utilization and effortless method transferability
- Uses standard quartz cuvettes and disposable vials
- Temperature controlled analysis of virtually all liquids or suspensions
- No sample preparation, no reagents, no waste
- Network-capable analyzer for centralized database management
- Hot-swappable modules that can be replaced in just a few minutes without performance loss.

The NIRS XDS RapidLiquid Analyzer, based on XDS near-infrared technology, provides the next generation of dedicated NIR systems for the rapid and nondestructive analysis of liquid chemical and pharmaceutical formulations. The NIRS XDS RapidLiquid Analyzer is designed to provide rapid quantitative and qualitative results for quality control and assurance.

The NIRS XDS RapidLiquid Analyzer is designed to provide rapid quantitative and qualitative results for quality control and assurance. With this Analyzer, virtually any liquid or suspension can be analyzed in both laboratory and atline situations. Samples are effortlessly analyzed in quartz cuvettes or disposable vials for trouble-free clean up. A temperature-controlled sample compartment provides the stable sample environment essential for precise measurements.

Only the XDS platform offers maximum system performance and instrument matching for decreased method development time, and effortless method transfer. Identification, qualitative and quantitative methods are easily implemented with the user-friendly, network-capable Vision® software. Precise and accurate analysis is accomplished with the press of a key or click of the mouse.



NIRS XDS RapidLiquid Analyzer

Ordering Information

2.921.1410 NIRS XDS RapidLiquid Analyzer

Fiber Optics – the flexible ones

The NIRS XDS Fiber Optics Analyzer family offers fiber optics modules for a wide variety of customer applications. The NIRS XDS SmartProbe Analyzer enables analyses of solids and liquids to be performed directly in shipping containers. Fiber optic probes attached to the NIRS XDS Interactance OptiProbe or to the NIRS XDS Transmission OptiProbe Analyzer also permit the use of laboratory instruments for scale-up and reaction monitoring. Solid or liquid samples can be analyzed using different probe types.

NIRS XDS SmartProbe Analyzer

With the NIRS XDS SmartProbe Analyzer, you can replace routine tests, expedite the production process and virtually eliminate quarantine time. The NIRS XDS SmartProbe Analyzer is ruggedly manufactured for either the warehouse or plant environments. The ergonomic, hand-held design is straightforward; simply place the probe in the sample and press the trigger. Pass/fail results are displayed on the handle after each test.

NIRS XDS Interactance OptiProbe Analyzer

With the NIRS XDS Interactance OptiProbe Analyzer, you receive both reflectance and immersion probes for a wide variety of sample types. The reflectance probe is used for scanning solids, highly scattering liquids and slurries. The immersion probe analyzes aqueous products, clear liquids and solvents. The fiber optics design of the NIRS XDS Interactance OptiProbe Analyzer allows it to be directly interfaced in difficult and hazardous sampling environments.

NIRS XDS Transmission OptiProbe Analyzer

With the NIRS XDS Transmission OptiProbe Analyzer, you can replace routine tests, expedite the production process, and minimize laboratory analysis times. The NIRS XDS Transmission OptiProbe Analyzer is designed for laboratory monitoring of aqueous products, clear liquids and solvents, as well as viscous samples. The NIRS XDS Transmission OptiProbe Analyzer is well-suited for scale-up process applications and atline measurements. Determinations of viscous samples can be carried out easily with this analyzer using disposable vials, thus reducing the amount of cleanup time to a minimum. With the optional Vial Heater Module, the system also provides automatic sample temperature equilibration prior to data analysis, thus increasing laboratory efficiency.



NIRS XDS SmartProbe Analyzer

Ordering Information

2.921.1510	NIRS XDS Interactance OptiProbe Analyzer
2.921.1520	NIRS XDS Transmission OptiProbe Analyzer
2.921.1530	NIRS XDS Transmission OptiProbe Analyzer – Heated Vials
2.921.1610	NIRS XDS SmartProbe Analyzer – 2 m Fiber
2.921.1620	NIRS XDS SmartProbe Analyzer – 3 m Fiber

Process analyzers

Introduction

NIR process analyzers offer information about chemical processes practically in real time, no matter how harsh the processing conditions may be. The process sample interface is dictated by the sample type and process conditions. Contact transmission and reflectance probes are used for analyzing clear to opaque liquids and solids.

Noncontact reflectance measurements are performed on materials transported in hoppers, transport and conveyor lines. Generally, NIR light from the instrument is transferred to the process sample interface using fiber optics. The number of fibers used in the fiber optic bundle is increased in order to maintain analytical performance as the light scattering properties of the process sample increase.

Single-fiber process NIR analyzers are typically employed to analyze clear liquids. Microbundle process NIR analyzers monitor slightly scattering liquid media, suspensions, and drying processes. Full-bundle process NIR analyzers are used for the most challenging of applications such as monitoring the drying of hydrated media or analyzing low-level constituents.

The length of the fiber optic interface can be from 1 m (large fiber bundle) to 150 m (single fiber optic). The use of longer fiber optic lengths enables a process analyzer to be set up outside of electrically classified or safety classified areas or under harsh operating conditions such as those with large temperature fluctuations. Up to nine separate process streams or sampling points can be monitored using a multiplexer NIR Process Analyzer from Metrohm NIRSystems. Multiplexing decreases both the costs per measuring point and the overall implementation costs for an NIR process analyzer.

Metrohm NIRSystems analyzers, software, application support and services meet a full range of process industry needs – process development, raw materials testing, process monitoring, endpoint determination, fluid bed drying, quality control and stability testing.

Fiber optic interface	Fiber size/count	Fiber length [m]	Sample type	Mode
Single fiber	600 μm , 1 illumination/1 collection	1–150	Clear liquids, thin films, gases	Transmission
Small fiber bundles	200 μm , 40 illumination/40 collection	1–75	Turbid liquids and suspensions	Transmission
Small fiber bundles	200 μm , 40 illumination/40 collection	1–75	Powders and films	Reflectance
Large fiber bundles	200 μm , 210 illumination/210 collection	1–15	Pastes, slurries, pellets, fibers	Reflectance

Comparison of fiber optic interface, fiber bundle size, and measurement mode. To maintain analytical performance, fiber count is increased as the turbidity of process sample increases.

NIRS XDS Process Analyzers – SingleFiber

- Direct inline measurement yields real-time analysis and data availability in seconds
- Interface made of simple optical fiber optimized for process streams, as with clear liquids and films
- Single-point or multiplex analyzer (four or nine sample channels)
- NEMA 4X/IP65 rated, ATEX ready
- Optional upgrade to hazardous area classification

The NIRS XDS Process Analyzer – SingleFiber belongs to the next generation of process analyzers for real-time analysis in the pharmaceutical and chemical industries. Nondestructive, accurate measurements are performed directly in the process line or in the reaction vessel.

Typical measurements include reaction monitoring and end point determination in refinery, petrochemical and polymer processes, solvent recovery in pharmaceutical API plants, and analysis of extruded polymer films and coatings. The use of single fiber optics and the associated probes and flow-through cells allows for cost-effective analysis of a wide variety of sample types ranging from clear liquids to transparent films.

The analyzer is available as a single-point or a multiplexer configuration. Two multiplexer process analyzer configurations offer up to either four or nine sampling points. This economical means of performing remote measurements enables the analyzer to be installed in an unrestricted area, reducing installation and operation costs. The patented, robust design of NIRS XDS Process Analyzers supplies a new level of consistent, dependable and reliable instrument performance and analysis while operating in harsh industrial environments.



NIRS XDS Process Analyzer

Ordering Information

- | | |
|------------|---|
| 2.928.0210 | NIRS XDS Process Analyzer – SingleFiber SinglePoint |
| 2.928.0220 | NIRS XDS Process Analyzer – SingleFiber 4 Channels |
| 2.928.0230 | NIRS XDS Process Analyzer – SingleFiber 9 Channels |

NIRS XDS Process Analyzers – MicroBundle

- Direct inline measurement for real-time analysis and data availability in seconds
- MicroBundle fiber optic interface, optimized for process stream: clear to opaque liquids, slurries, suspensions and powders
- One sample channel or multiplexing of up to nine channels
- Fiber to analyzer connection via SMA fittings
- NEMA 4X/IP65 rated, ATEX ready
- Optional upgrade to hazardous area classification

The NIRS XDS Process Analyzer – MicroBundle belongs to the next generation of process analyzers for real-time analysis in the pharmaceutical and chemical industries. Nondestructive, accurate measurements are performed directly in the process line, granulator, dryer or reaction vessel.

Process analyzers are used throughout the process stream to ensure optimum performance for many types of samples. The multi-fiber bundles used allow for cost-effective analysis of sample types ranging from clear liquids to suspensions and solids. Configure the analyzer

with a reflectance probe, an immersion probe or a transmission probe pair for an optimized interface to your particular sample type.

The XDS Process Analyzer – MicroBundle is available as a single-point or a multiplexer configuration for measurement of up to either four or nine sampling points. This economical means of performing remote measurements enables the analyzer to be installed in an unrestricted area, reducing installation and operation costs.

The patented, robust design of NIRS XDS Process Analyzers supplies a new level of consistent, dependable and reliable instrument performance and analysis while operating in harsh industrial environments. Monitoring with near-infrared (NIR) fits in well with Process Analytical Technology (PAT) initiatives as proposed by the FDA.



NIRS XDS Process Analyzer

Ordering Information

- | | |
|------------|---|
| 2.928.0110 | NIRS XDS Process Analyzer – MicroBundle SinglePoint |
| 2.928.0120 | NIRS XDS Process Analyzer – MicroBundle 4 Channels |
| 2.928.0130 | NIRS XDS Process Analyzer – MicroBundle 9 Channels |

NIRS XDS Process Analyzer – DirectLight/NonContact

- Nondestructive inline near-infrared analysis (NIR) of the moving product
- Noncontact reflectance measurements directly in the product line
- Utilization above conveyor belts, webs for homogeneous or nonhomogeneous products
- Wavelength range from 800 to 2,200 nm
- NEMA 4X/IP65 rated, measuring head IP69K stainless steel

Based on NIR XDS technology, the NIRS XDS Process Analyzer – DirectLight/NonContact is numbered among the next generation of noncontact process analyzers for real-time analysis. Nondestructive, accurate measurements are performed wherever a product is moving and accessible, for instance, above a conveyor belt, web or sheet.

Noncontact reflectance measurement can provide more detailed chemical analysis for loose to densely packed, homogeneous or nonhomogeneous solid products. Noncontact measurement is used for quality control of fibers, sheets, laminates, and web-based products like plastics,

papers, and textiles. The measuring head is attached at the terminal end of an optical fiber. A high-intensity light source contained in the sensor head illuminates the sample. Light interacts with the sample and is reflected back to the sensor head, picked up by the collection fiber bundle, and passed on to the instrument for dispersion and signal detection. The patented, robust design of the NIRS XDS Process Analyzers supplies a higher level of consistent, reliable instrument performance and analysis for operation in harsh chemical environments.



NIRS XDS Process Analyzer

Ordering Information

2.928.0310 NIRS XDS Process Analyzer –
DirectLight/NonContact

NIRS Analyzer PRO

The NIRS Analyzer PRO is a process analyzer based on high-resolution diode array technology. It provides non-destructive analysis of products such as granules, powders, slurries, or opalescent substances directly in the process line without bypass.

The analyzer is housed in a robust cabinet mounted at the relevant location in the production area. Measurements are displayed in the control room and results can be fed into a regulation system for closed-loop automatic control. Additionally, the analyzer helps to optimize the use of raw materials and to run production consistently closer to target specifications. Accurate instrument adjustment enhances method development, minimizes implementation requirements and ensures calibration model transferability between analyzers.

The NIRS Analyzer PRO is available with dedicated interfaces based on reflectance or transmittance technology whichever is best suited for each application area. Measurements are done directly on the moving sample in the process stream. A high-intensity dual-lamp light source illuminates the sample directly or through an optical

fiber. The light interacts with the sample and the reflected or transmitted light is measured by the diode array sensor. The backup lamp in the dual-lamp system secures uptime and analytical accuracy is unchanged even after switching to a new lamp.

The complete wavelength range is measured instantaneously enabling measurements also on fast moving samples with high accuracy. Calibrations are transferable between instruments, ensuring easy expansion to other measuring points. Integration to process regulations systems can be done through the Metrohm OPC interface.

ContactReflection

Inline analyses of pastes, granules, powders, etc. in pipes or transport systems without bypass can be performed. The products pass over the interface window. The window reflection interface can easily be installed into the production line either by using flow-through cells or by welding an interface flange into the wall of the pipe/transport system.

FiberSystem

Process streams of clear to opaque liquids, slurries, suspensions and powders can be measured and optimized inline with this system. Depending on the sample type, the analyzer can be configured with fiber optic Micro-Bundle reflection or immersion probes.

DirectLight/NonContact

Inline analysis of products where direct contact with the product is not a technically feasible solution, i.e., products transported on a conveyor belt.



NIRS Analyzer PRO

Ordering Information

2.928.1110	NIRS Analyzer PRO – ContactReflection
2.928.1120	NIRS Analyzer PRO – FiberSystem
2.928.1130	NIRS Analyzer PRO – DirectLight/ NonContact



Ion chromatography



Ion chromatography

Professional IC Vario – Systems	134	Professional IC Vario – Instruments	177
940 Professional IC Vario systems – Introduction	134	940 Professional IC Vario instruments – Introduction	177
Professional IC – ProfIC Vario systems	135	940 Professional IC Vario – Overview	178
How to find the right ProfIC Vario system	136	940 Professional IC Vario ONE	179
„ProfIC Vario 1 Cation“	137	940 Professional IC Vario ONE/Prep 1	179
„ProfIC Vario 2 Cation“	138	940 Professional IC Vario ONE/Prep 2	179
Metrohm Inline Ultrafiltration and Dialysis	139	940 Professional IC Vario ONE/HPG	179
„ProfIC Vario 3 Cation“	140	940 Professional IC Vario ONE/LPG	180
„ProfIC Vario 4 Cation“	141	940 Professional IC Vario ONE/ChS	180
„ProfIC Vario 5 Cation“	142	940 Professional IC Vario ONE/ChS/HPG	180
„ProfIC Vario 6 Cation“	143	940 Professional IC Vario ONE/ChS/LPG	180
„ProfIC Vario 7 Cation“	144	940 Professional IC Vario ONE/ChS/PP	181
„ProfIC Vario 8 Cation“	145	940 Professional IC Vario ONE/ChS/PP/HPG	181
„ProfIC Vario 9 Cation“	146	940 Professional IC Vario ONE/ChS/PP/LPG	181
„ProfIC Vario 14 Cation“	147	940 Professional IC Vario ONE/SeS	181
„ProfIC Vario 15 Cation“	148	940 Professional IC Vario ONE/SeS/Prep 1	182
„ProfIC Vario 1 Anion“	149	940 Professional IC Vario ONE/SeS/Prep 2	182
„ProfIC Vario 1 Anion DR“	150	940 Professional IC Vario ONE/SeS/Prep 3	182
Suppression repeatability	151	940 Professional IC Vario ONE/SeS/HPG	182
Sequential suppression	152	940 Professional IC Vario ONE/SeS/LPG	183
„ProfIC Vario 2 Anion“	153	940 Professional IC Vario ONE/SeS/PP	183
„ProfIC Vario 3 Anion“	154	940 Professional IC Vario ONE/SeS/PP/Prep 1	183
„ProfIC Vario 4 Anion“	155	940 Professional IC Vario ONE/SeS/PP/Prep 2	183
„ProfIC Vario 5 Anion“	156	940 Professional IC Vario ONE/SeS/PP/Prep 3	184
„ProfIC Vario 6 Anion“	157	940 Professional IC Vario ONE/SeS/PP/HPG	184
„ProfIC Vario 7 Anion“	158	940 Professional IC Vario ONE/SeS/PP/LPG	184
„ProfIC Vario 8 Anion“	159	940 Professional IC Vario TWO	184
„ProfIC Vario 9 Anion“	160	940 Professional IC Vario TWO/ChS	185
„ProfIC Vario 10 Anion“	161	940 Professional IC Vario TWO/ChS/PP	185
„ProfIC Vario 11 Anion“	162	940 Professional IC Vario TWO/SeS	185
„ProfIC Vario 12 Anion“	163	940 Professional IC Vario TWO/SeS/PP	185
„ProfIC Vario 14 Anion“	164	Professional IC Vario – Detectors	186
„ProfIC Vario 15 Anion“	165	IC Conductivity Detector	186
„ProfIC Vario 1 Amperometry“	166	IC Amperometric Detector	186
„ProfIC Vario 1 UV/VIS“	167	944 Professional UV/VIS Detector Vario	186
„ProfIC Vario 1 PCR-UV/VIS“	168	945 Professional Detector Vario – Conductivity	186
„ProfIC Vario 1 AnCat“	169	945 Professional Detector Vario – Amperometry	187
„ProfIC Vario 2 AnCat“	170	945 Professional Detector Vario – Conductivity &	
„ProfIC Vario 4 AnCat“	171	Amperometry	187
„ProfIC Vario 5 AnCat“	172	Inline Eluent Preparation – Introduction	188
„ProfIC Vario 6 AnCat“	173	941 Eluent Production Module	189
„ProfIC Vario 9 AnCat“	174		
„ProfIC Vario 14 AnCat“	175		
„ProfIC Vario 15 AnCat“	176		

Extension Module Vario – Overview	190	Professional IC Vario – Hyphenated systems	204
942 Extension Module Vario Prep 2	191	IC Vario coupling techniques – Introduction	204
942 Extension Module Vario HPG	191	TitriC Vario pro I	205
942 Extension Module Vario LQH	191	TitriC Vario pro II	205
942 Extension Module Vario ChS/PP	191	TitriC Vario pro III	205
942 Extension Module Vario SeS/PP	192	VoltIC Vario pro I	205
942 Extension Module Vario ONE/Deg	192	930 Metrohm Combustion IC	206
		920 Absorber Module	206
Compact IC Flex – Instruments	193	MMS 5000 Autosampler	206
Compact IC Flex – Introduction	193	Combustion Module (Oven + ABD)	206
Compact IC Flex – Overview	194	Auto Boat Drive	207
930 Compact IC Flex	195	LPG/GSS Module	207
930 Compact IC Flex Deg	195	Combustion Module (Oven + LPG/GSS)	207
930 Compact IC Flex ChS	195	PILS, Particle Into Liquid Sampler	207
930 Compact IC Flex ChS/Deg	195	MARGA	208
930 Compact IC Flex ChS/PP	196		
930 Compact IC Flex ChS/PP/Deg	196	Automation in ion chromatography	209
930 Compact IC Flex SeS	196	Overview of IC automation	209
930 Compact IC Flex SeS/Deg	196	858 Professional Sample Processor	210
930 Compact IC Flex SeS/PP	197	858 Professional Sample Processor – Pump	210
930 Compact IC Flex SeS/PP/Deg	197	858 Professional Sample Processor – Pump –	
930 Compact IC Flex Oven	197	Injector	210
930 Compact IC Flex Oven/Deg	197	919 IC Autosampler plus	210
930 Compact IC Flex Oven/ChS	198	863 Compact IC Autosampler	211
930 Compact IC Flex Oven/ChS/Deg	198	815 Robotic Soliprep for LC	211
930 Compact IC Flex Oven/ChS/PP	198	889 IC Sample Center	211
930 Compact IC Flex Oven/ChS/PP/Deg	198	889 IC Sample Center – cool	211
930 Compact IC Flex Oven/SeS	199	Additional Sample Processors for IC	212
930 Compact IC Flex Oven/SeS/Deg	199		
930 Compact IC Flex Oven/SeS/PP	199		
930 Compact IC Flex Oven/SeS/PP/Deg	199		
Basic IC plus – Instruments	200		
883 Basic IC plus	200		
883 Basic IC plus Package	200		
Additional IC Vario components	201		
Alternative IC components – Introduction	201		
Heatable reactors and column compartments	202		
943 Professional Reactor Vario	202		
943 Professional Thermostat Vario	202		
Data Converters	203		
771 IC Compact Interface	203		
771 IC Compact Interface; MagIC Net Professional	203		
771 IC Compact Interface; MagIC Net Compact	203		
891 Professional Analog Out	203		

Liquid Handling in ion chromatography	213
Liquid Handling in IC – Introduction	213
800 Dosino	214
846 Dosing Interface	214
IC equipment: Additional eluent on the Eluent Production Module	214
IC equipment: Inline dialysis	214
IC equipment: Inline ultrafiltration	215
IC equipment: Inline dilution	215
IC equipment: Liquid Handling Station, left	215
IC equipment: MiPCT	215
IC equipment: Dose-in Gradient	216
IC equipment: MiPCT-ME	216
IC equipment: MiPUT	216
IC equipment: MiPT	216
IC equipment: Dosino regeneration	217
IQ/OQ Kit for IC	217
IC equipment for Liquid Handling Set for PILS Peristaltic pump, 8-channel	217
Professional Vario IC – Software	218
MagIC Net – Introduction	218
MagIC Net 3.0 Compact CD: 1 license	219
MagIC Net 3.0 Professional CD: 1 license	219
MagIC Net 3.0 Multi CD: 3 licenses	219
Metrohm IC Driver for Empower	219

Professional IC Vario – Systems

940 Professional IC Vario systems – Introduction

Intelligent ion chromatography

The 940 Professional IC Vario is the second generation of professional ion chromatography systems with intelligent system components that are optimally coordinated with one another. The path from the sample to the precise result has become simpler, as the system itself is thinking during the procedure and even making logical decisions.

- Intelligence in the hardware of the 940 Professional IC Vario:
 - **iPump**
 - **iDetector**
 - **iReactor**
 - **iCell**
 - **intelligent Dosino**
- Intelligence in the **MagIC Net** software
- Intelligence in the Metrosep **iColumns**

These are the intelligent system components that monitor all functions, optimize them and, if desired, also document them in accordance with FDA requirements. The configuration of the system is as simple as possible, as the components log in automatically and make all relevant information available to the MagIC Net soft-


ware. Optimum operation of the 940 Professional IC Vario and the results are both monitored. If a parameter lies outside of the specified range, then the user will be informed via e-mail or SMS. The 940 Professional IC Vario is a complex and very high-performance system for which simple and intuitive operation is provided by the MagIC Net software. This applies for experienced users with complex applications and sophisticated calculations as well as for users who value „one-button operation“. Every user level is possible. Innovation, flexibility and exceptionally simple operation result from the intelligence of the 940 Professional IC Vario, the 942 Extension Module Vario, the 858 Professional Sample Processor and the MagIC Net software.

Online configurator

With just a few mouseclicks, this software tool can be used to configure any imaginable IC system down to the last detail. The path to the tailored solution for individual requirements in ion chromatography has thus become even simpler.

It is precisely here that the new online configurator provides the user with support. Starting from the analysis requirements, the user selects the necessary modules from the comprehensive ion chromatography array on offer from Metrohm and specifies a system, step by step, that optimally meets his requirements. Once the solution has been specified down to the last detail, the user can print out „his“ system as a photo-realist graph in PDF format. In addition, he receives a detailed list of the modules and components contained in the respective system along with their order numbers.

Access to the new online configurator is through ic940.metrohm.com

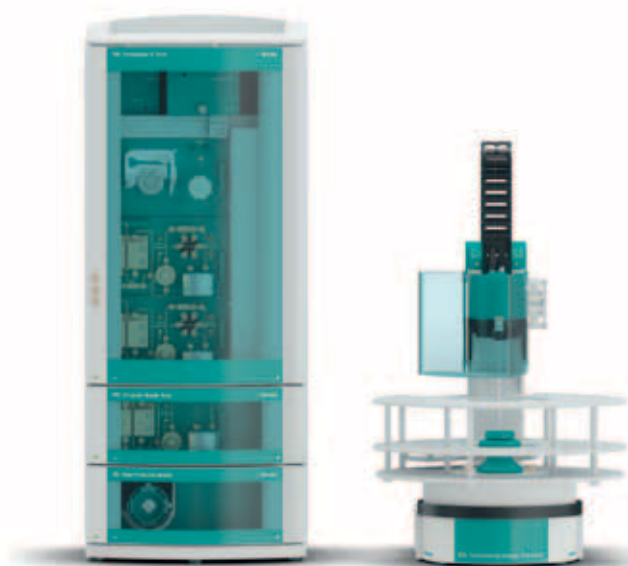

Professional IC – ProfIC Vario systems


The „ProfIC Vario“ systems are assemblies of Professional IC instruments and accessory parts that are custom-tailored for a particular application group. These systems contain all of the components required to perform the respective application with complete automation. The main components are:

- **940 Professional IC Vario**
- **IC Conductivity Detector**
- **IC Amperometric Detector**
- **944 Professional UV/VIS Detector Vario**
- **945 Professional Detector Vario**
- **858 Professional Sample Processor**
- **942 Extension Module Vario**
- **800 Dosino**

In the respectively required versions with the corresponding accessory parts. Not included in the scope of delivery are the separation column, suppressor rotor, MagIC Net, the sample rack and the sample vessels. This ensures the greatest possible flexibility of the systems.

No matter whether it be determination of anions in the analytical service laboratory with very high sample throughput or the detection of cations in the ultratrace range, as is required in nuclear power plants, the ProfIC Vario systems offer customized solutions for even the most sophisticated measurements in ion chromatography. 37 systems can be called up at www.metrohm.com/com/Produkte2/IC/ProfIC-Vario-Systems.html.

How to find the right ProfIC Vario system

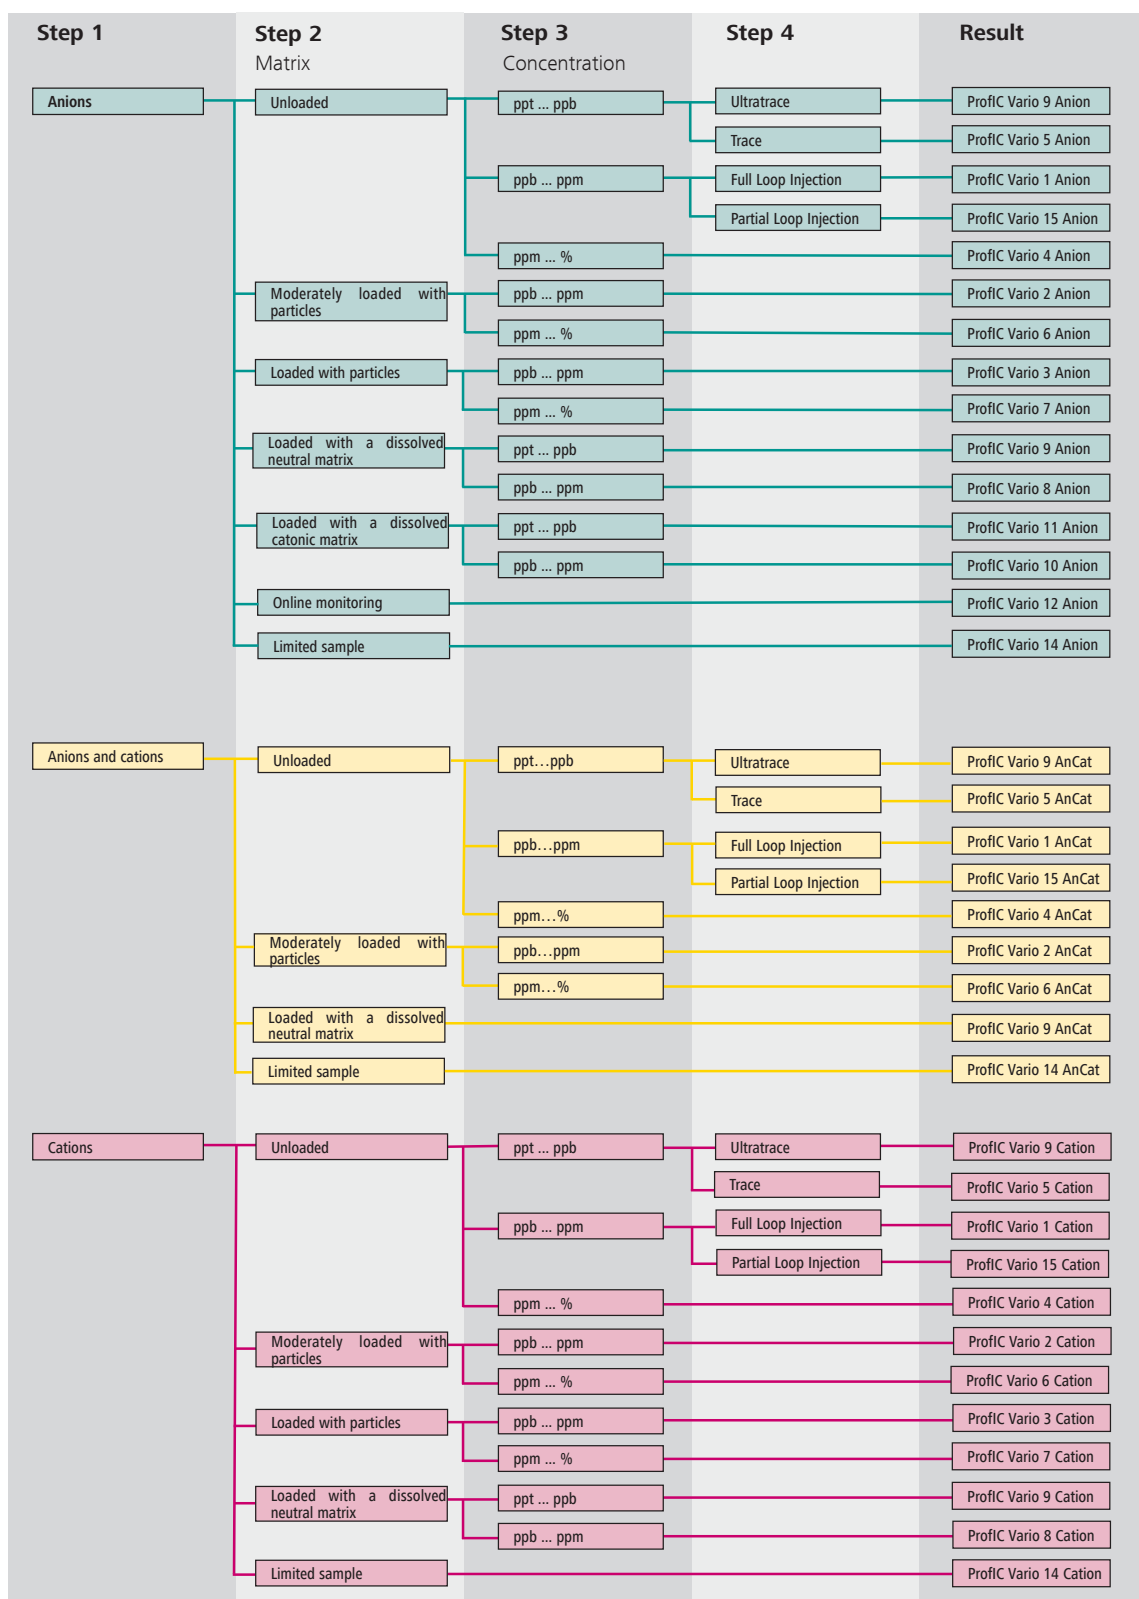

„ProfIC Vario 1 Cation“ – Professional IC Vario system for automated ion chromatography

The Professional IC Vario system with **direct conductivity detection** enables the fully automated determination of cations or anions (non-suppressed).

Typical areas of application:

- Universal application for cation analysis
- Routine analysis with large numbers of samples without additional sample preparation
- Coupling with MS or ICP/MS instruments for research and development tasks

The „ProfIC Vario 1 Cation“ is comprised of the 940 Professional IC Vario ONE, one „iDetector“ intelligent conductivity detector and one 858 Professional Sample Processor.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

Technical Information


Parts

- 1 x 2.940.1100 940 Professional IC Vario ONE
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor

The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- MagIC Net

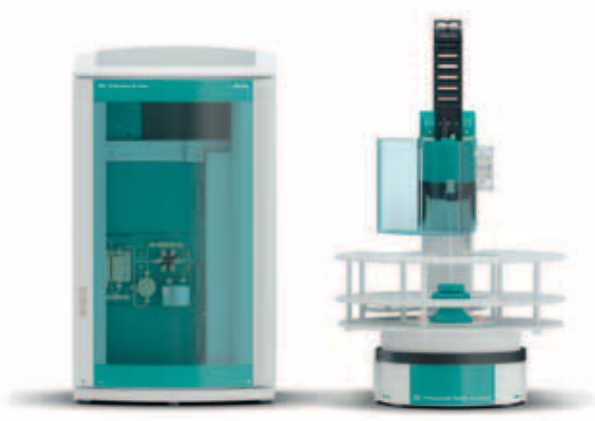

„ProfIC Vario 1 Cation“

Ordering Information

ProfIC Vario 1 Cation

„ProfIC Vario 2 Cation“ – Professional IC Vario system with Inline Ultrafiltration

The Professional IC Vario system with **Metrohm Inline Ultrafiltration** and **conductivity detection** enables the fully automatic determination of cations or anions (non-suppressed).

Typical areas of application:

- Samples with slight to medium-severe loads of particles, algae or bacteria
- Drinking and surface water
- Process and waste water

The „ProfIC Vario 2 Cation“ is comprised of one 940 Professional IC Vario ONE, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor and an IC equipment for Inline Ultrafiltration.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

Technical Information

Parts


- 1 x 2.940.1100 940 Professional IC Vario ONE
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 6.5330.110 IC equipment: Inline Ultrafiltration

The IC equipment for Inline Ultrafiltration contains all of the parts needed for integrating Metrohm Inline Ultrafiltration in the system.

Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor. A minimum of 5 mL of sample is required for the Inline Ultrafiltration.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- MagIC Net

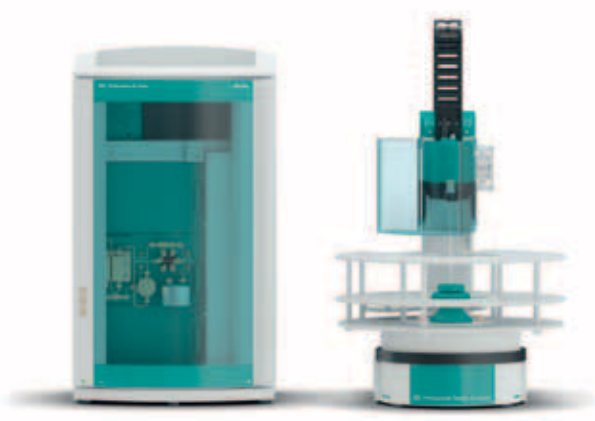

„ProfIC Vario 2 Cation“


Ordering Information

ProfIC Vario 2 Cation

Metrohm Inline Ultrafiltration and Dialysis

Metrohm Inline Ultrafiltration


In modern ion chromatography, it is recommended that all samples be filtered before injection. Separation columns with particle sizes of less than 10 µm require absolutely particle-free sample solutions. Unfiltered solutions can lead to pressure increases on the column and thus to a certain extent to a massively shortened lifetime for the separation column. The usual manual filtration takes place with disposable filter cartridges with pore sizes of 0.45 µm or smaller. These become blocked very quickly, particularly with samples containing minuscule particles. As an alternative, sample changers are also used with filter caps. Here the pore size is often larger than it is with the disposable filters. These are expensive and there is also a danger of blockage associated with them. These problems are a thing of the past with Metrohm Inline Ultrafiltration, a membrane separation technique. The samples are placed directly on the turntable. The sample stream is guided into the lower chamber of the ultrafiltration cell and along the membrane to the waste container at the time the samples are processed. The peristaltic pump generates an underpressure in the upper chamber of the cell, thus causing the sample solution to be suctioned through the ultrafiltration membrane. The filtered sample solution reaches the injection loop and is subsequently injected. Less than 20% of the original solution is removed as filtrate, the remainder flows directly into the waste. The formation of a filter cake that could lead to a jamming of the membrane is largely prevented by this and by the geometric alignment of the cell. Metrohm Inline Ultrafiltration is especially suitable for samples with small to medium loads, e.g., drinking water, surface water, sewage, digestion solutions, extractions.

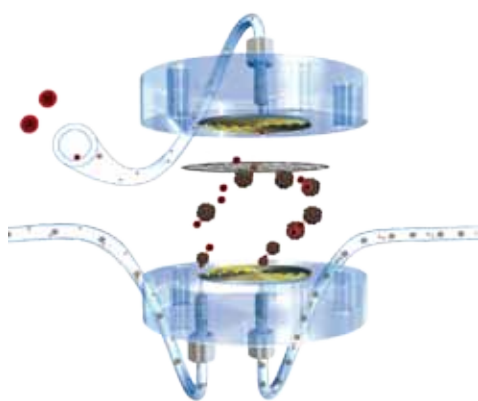

Ultrafiltration

Metrohm Inline Dialysis

More severely loaded samples require complex and work-intensive preparatory steps prior to their actual determination. For this, Metrohm Inline Dialysis permits a significant rationalization of the entire analysis. The only condition the sample must meet: It must be present in liquid form or be able to be transformed into one and be largely homogenous. Larger-sized particles are also to be removed with centrifuging. Afterwards, the sample solution is dialyzed in the dialysis cell in accordance with the method patented by Metrohm (European Patent 0 820 804, US Patent 5,861,097). Practically complete dialysis is achieved, thanks to this special „Inline Stopped Flow Dialysis“ method. That means that the acceptor solution exhibits the same ion concentration as the original sample (equilibrium dialysis). Afterwards, the acceptor solution is injected directly into the ion chromatograph and analyzed. In the case of ultrafiltration, a pressure differential causes the sample solution to be filtered through the membrane, but with dialysis it is the difference in concentration between the two sides that is the driving force. The ions to be determined diffuse through the membrane, but no sample solution is pressed through the membrane. Accordingly, no filter cake is formed that could block the membrane. With the aid of this technology, it is possible to determine anions and cations, even in cutting oil emulsions, biodiesel, milk products or bodily fluids such as blood and urine. If the system is programmed in such a way that the next sample is dialyzed during the current run, then the total analysis time corresponds to that of a direct injection.

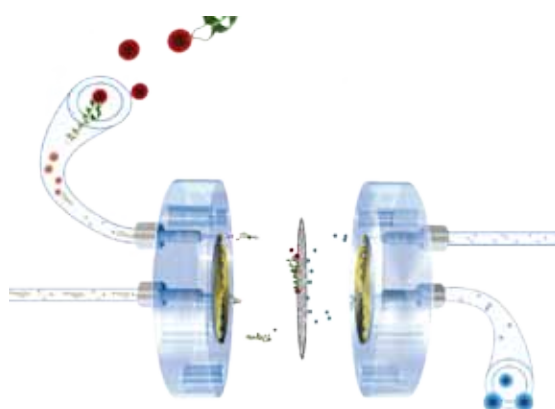

«Stopped flow» method. An equilibrium is achieved between the acceptor solution and the sample solution

„ProfIC Vario 3 Cation“ – Professional IC Vario system with Inline Dialysis

The Professional IC Vario system with **Metrohm inline dialysis** and **conductivity detection** enables the fully automatic determination of cations or anions (non-suppressed).

Typical areas of application:

- Samples with severe loads of particles, algae or bacteria
- Process, wash and waste water
- Emulsions, dispersions, cutting oils and samples containing petroleum
- Milk products and other samples containing protein

The „ProfIC Vario 3 Cation“ is comprised of one 940 Professional IC Vario ONE/Prep 1, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor and one IC equipment for Inline Dialysis.

The 940 Professional IC Vario ONE/Prep 1 is equipped with the „ONE“ and „Prep 1“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive,

Technical Information

Parts

- 1 x 2.940.1110 940 Professional IC Vario ONE/Prep 1
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 6.5330.100 IC equipment: Inline Dialysis

column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

In addition, a bidirectional two-channel peristaltic pump for sample preparation or sample injection is located in the lower segment of the instrument („Prep 1“). The position for the installation of the dialysis cell is prepared here.

The IC equipment for Inline Dialysis contains all of the parts required for the Metrohm-patented „Inline Stopped Flow Dialysis“.


Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor. At least 10 mL of sample are required for Inline Dialysis.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- MagIC Net

Ordering Information

ProfIC Vario 3 Cation

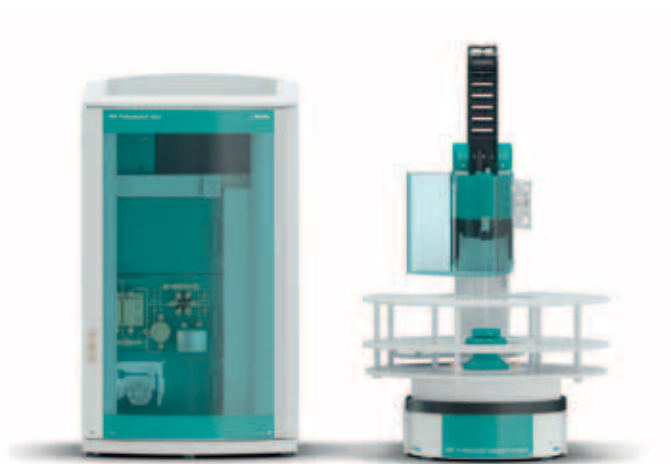

„ProfIC Vario 3 Cation“

„ProfIC Vario 4 Cation“ – Professional IC Vario system with Inline Dilution

The Professional IC Vario system with **Metrohm's intelligent Inline Dilution** and **conductivity detection** enables the fully automatic determination of cations or anions (non-suppressed) in concentrated solutions.

Typical areas of application:

- Samples with high ion concentration
- Samples from all industries

The „ProfIC Vario 4 Cation“ is comprised of one 940 Professional IC Vario ONE, one „iDetector“ intelligent conductivity detector, one 741 Magnetic Stirrer, one 800 Dosino and one IC equipment for Inline Dilution.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

Technical Information

Parts

1 x 2.940.1100 940 Professional IC Vario ONE
1 x 2.850.9010 IC Conductivity Detector
1 x 2.858.0020 858 Professional Sample Processor
1 x 2.741.0010 741 Magnetic Stirrer
1 x 2.800.0010 800 Dosino
1 x 6.5330.120 IC equipment: Inline Dilution

The „ProfIC Vario 4 Cation“ offers the option of automated inline dilution of every sample. This takes place at an external position on the 858 Professional Sample Processor. The 800 Dosino aspirates the volume to be diluted into the transfer tubing, doses it into the Liquid Handling Station and adds the required volume of dilution medium. All of the parts required are on hand with the IC equipment for Inline Dilution.


The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- MagIC Net

Ordering Information

ProfIC Vario 4 Cation

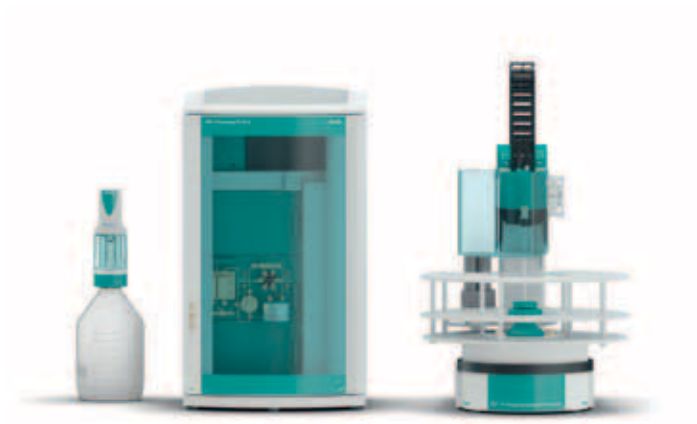

„ProfIC Vario 4 Cation“

„ProfIC Vario 5 Cation“ – Professional IC Vario system with Metrohm’s intelligent preconcentration technique (MiPCT)

The Professional IC Vario system with **Metrohm’s intelligent inline sample preconcentration** and **conductivity detection** enables the fully automatic determination of cations or anions (non-suppressed) in solutions with low ion concentration.

Typical areas of application:

- Numerous applications, ranging from ultrapure water analysis to drinking water analysis
- Analyses of different samples from power plants
- Process control and monitoring of rinsing solutions, e.g., in the semiconductor industry

The „ProfIC Vario 5 Cation“ is comprised of one 940 Professional IC Vario ONE, one „iDetector“ intelligent conductivity detector, one 800 Dosino, one 858 Professional Sample Processor and one IC equipment for MiPCT.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection

Technical Information

Parts

- 1 x 2.940.1100 940 Professional IC Vario ONE
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0010 858 Professional Sample Processor
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.140 IC equipment: MiPCT

valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

With the 800 Dosino and the IC equipment for MiPCT, all of the parts required for Metrohm’s intelligent preconcentration technique are on hand.


The 858 Professional Sample Processor makes the samples available. The transfer takes place with the 800 Dosino. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- MagIC Net

Ordering Information

ProfIC Vario 5 Cation

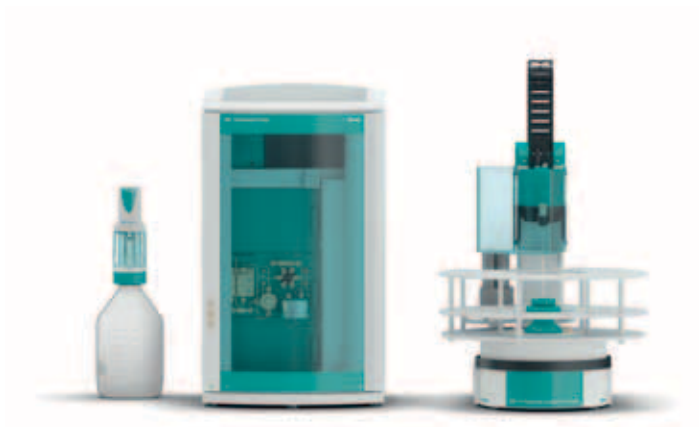

„ProfIC Vario 5 Cation“

„ProfIC Vario 6 Cation“ – Professional IC Vario system with Inline Dilution and Inline Ultrafiltration

The Professional IC Vario system with **Metrohm Inline Dilution**, **Metrohm Inline Ultrafiltration** and **conductivity detection** enables the fully automatic determination of cations or anions (non-suppressed) that are present in very high concentrations and that have matrices containing particles.

Typical areas of application:

- Rinse, process and waste water
- Extractions and digestion solutions
- Food samples

The „ProfIC Vario 6 Cation“ is comprised of one 940 Professional IC Vario ONE, one „iDetector“ intelligent conductivity detector, one 741 Magnetic Stirrer, one 800 Dosino, one 858 Professional Sample Processor, an IC equipment for Inline Dilution and an IC equipment for Inline Ultrafiltration.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection

Technical Information

Parts

- 1 x 2.940.1100 940 Professional IC Vario ONE
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 2.741.0010 741 Magnetic Stirrer
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.120 IC equipment: Inline Dilution
- 1 x 6.5330.110 IC equipment: Inline Ultrafiltration

valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

The „ProfIC Vario 6 Cation“ offers the option of automated inline dilution of every sample. This takes place at an external position on the 858 Professional Sample Processor. The 800 Dosino aspirates the volume to be diluted into the transfer tubing, doses it into the Liquid Handling Station and adds the required volume of dilution medium. All of the parts required are on hand with the IC equipment for Inline Dilution.

The IC equipment for Inline Ultrafiltration contains all of the parts needed for integrating the subsequent Metrohm Inline Ultrafiltration in the system.


The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- MagIC Net

Ordering Information

ProfIC Vario 6 Cation

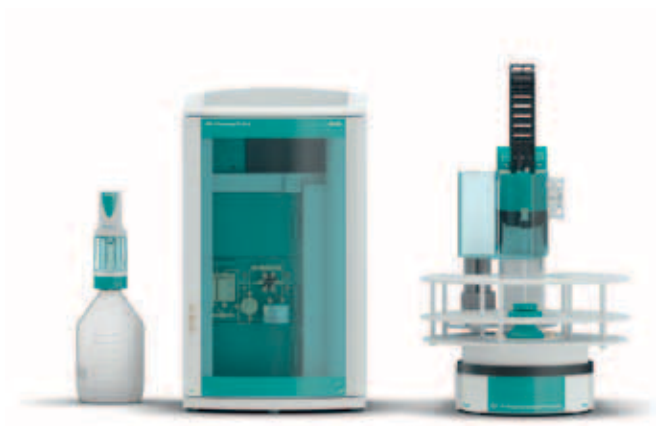

„ProfIC Vario 6 Cation“

„ProfIC Vario 7 Cation“ – Professional IC Vario system with Inline Dilution and Inline Dialysis

The Professional IC Vario system with **Metrohm Inline Dilution, Inline Dialysis** and **conductivity detection** enables the fully automated determination of cations or anions (non-suppressed) that are present in high concentrations and in difficult matrices.

Typical areas of application:

- Process, wash and waste water
- Samples containing oil
- Inline Extraction for biodiesel analysis

The „ProfIC Vario 7 Cation“ is comprised of one 940 Professional IC Vario ONE/Prep 1, one „iDetector“ intelligent conductivity detector, one 741 Magnetic Stirrer, one 800 Dosino, one 858 Professional Sample Processor, an IC equipment for Inline Dilution and an IC equipment for Inline Dialysis.

The 940 Professional IC Vario ONE/Prep 1 is equipped with the „ONE“ and „Prep 1“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive,

Technical Information

Parts

1 x 2.940.1110	940 Professional IC Vario ONE/Prep 1
1 x 2.850.9010	IC Conductivity Detector
1 x 2.858.0020	858 Professional Sample Processor
1 x 2.741.0010	741 Magnetic Stirrer
1 x 2.800.0010	800 Dosino
1 x 6.5330.120	IC equipment: Inline Dilution
1 x 6.5330.100	IC equipment: Inline Dialysis

column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

In addition, a bidirectional two-channel peristaltic pump for sample preparation or sample injection is located in the lower segment of the instrument („Prep 1“). The position for the installation of the dialysis cell is prepared here.

The „ProfIC Vario 7 Cation“ offers the option of automated inline dilution of every sample. This takes place at an external position on the 858 Professional Sample Processor. The 800 Dosino aspirates the volume to be diluted into the transfer tubing, doses it into the Liquid Handling Station and adds the required volume of dilution medium. All of the parts required are on hand with the IC equipment for Inline Dilution.

The IC equipment for Inline Dialysis contains all of the parts required for the subsequent Metrohm-patented „Inline Stopped Flow Dialysis“.

The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- MagIC Net

Ordering Information

ProfIC Vario 7 Cation



„ProfIC Vario 7 Cation“

„ProfIC Vario 8 Cation“ – Professional IC Vario system with Inline Matrix Elimination

The Professional IC Vario system with **Metrohm Inline Matrix Elimination** and **conductivity detection** enables the determination of cations or anions (non-suppressed) in difficult matrices.

Typical areas of application:

- Trace analysis in polar solvents
- Quality controls in fuels, fuel mixtures and biofuels
- Quality management of chemicals

The „ProfIC Vario 8 Cation“ is comprised of one 940 Professional IC Vario ONE, one „iDetector“ intelligent conductivity detector and one 858 Professional Sample Processor.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

Technical Information


Parts

1 x 2.940.1100	940 Professional IC Vario ONE
1 x 2.850.9010	IC Conductivity Detector
1 x 2.858.0030	858 Professional Sample Processor
1 x 6.1602.150	Bottle attachment / GL 45 - 3 x UNF
1 x 6.1608.070	Eluent bottle / 2 L / GL 45
1 x 6.1825.230	PEEK sample loop 10 µL

The injector and the peristaltic pump on the 858 Professional Sample Processor and the additional accessory parts enable Inline Matrix Elimination. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor. As a rule, only small volumes with a maximum of 1 mL sample are required for matrix elimination.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- MagIC Net

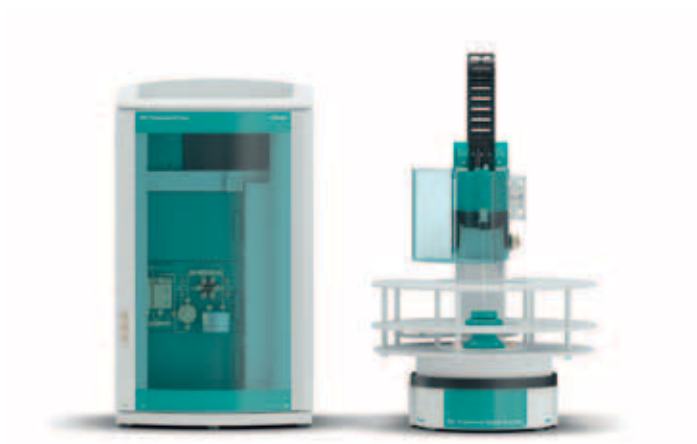

„ProfIC Vario 8 Cation“

Ordering Information

ProfIC Vario 8 Cation

„ProfIC Vario 9 Cation“ – Professional IC Vario system with Metrohm’s intelligent preconcentration technique and Inline Matrix Elimination (MiPCT-ME)

The Professional IC Vario system with **Metrohm’s intelligent inline preconcentration technique, Inline Matrix Elimination** and **conductivity detection** enables ultratrace analysis down to the lowest ppt range (ng/L) of cations in complex matrices.

Typical areas of application:

- Ultratrace analysis in samples from nuclear power plants and conventional power plants
- Trace and ultratrace analysis in extraction agents and organics
- Trace analysis in snow and ice

The „ProfIC Vario 9 Cation“ is comprised of one 940 Professional IC Vario ONE, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor, two 800 Dosinos and one IC equipment for MiPCT-ME.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection

Technical Information

Parts

- 1 x 2.940.1100 940 Professional IC Vario ONE
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0010 858 Professional Sample Processor
- 2 x 2.800.0010 800 Dosino
- 1 x 6.5330.160 IC equipment: MiPCT-ME

valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

The two 800 Dosinos and the IC equipment for MiPCT-ME enable preconcentration of the sample and subsequent matrix elimination. Typical preconcentration volumes are 4 - 4,000 µL.

The 858 Professional Sample Processor makes the samples available. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- MagIC Net



„ProfIC Vario 9 Cation“

Ordering Information

ProfIC Vario 9 Cation

„ProfIC Vario 14 Cation“ – Professional IC Vario system with Metrohm’s intelligent Pick-up-Injection Technique (MiPuT)

The Professional IC Vario system with **Metrohm’s intelligent Pick-up Injection Technique (MiPuT)** and **conductivity detection** enables the determination of cations or anions (non-suppressed) from the smallest of sample volumes.

Typical areas of application:

- For universal application for all types of samples when only small sample quantities are available
- Investigation of biochemical processes
- Environmental sample extracts

The „ProfIC Vario 14 Cation“ is comprised of one 940 Professional IC Vario ONE, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor, one 800 Dosino and one IC equipment for MiPuT.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for

Technical Information

Parts

- 1 x 2.940.1100 940 Professional IC Vario ONE
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.170 IC equipment: MiPuT


cooling and heating two iColumns and an external column position in the room temperature range.

The 800 Dosino and the IC equipment for MiPuT enable Metrohm’s intelligent Pick-up Injection Technique. 2 - 50 µL of the samples can be removed and injected directly.

Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack (recommended 6.2041.480 Sample rack 159 x 2 mL + 3 x 300 mL)
- MagIC Net

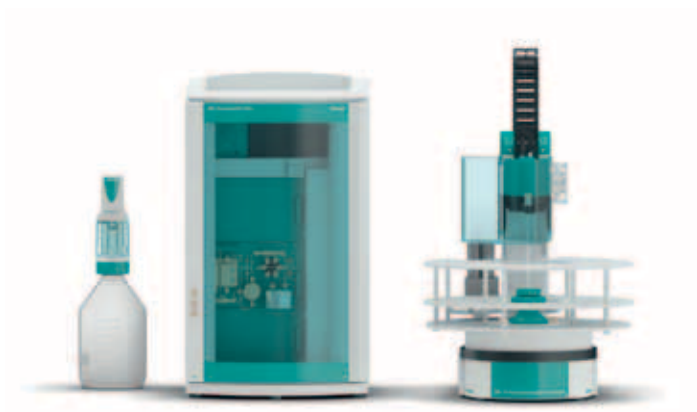

„ProfIC Vario 14 Cation“

Ordering Information

ProfIC Vario 14 Cation

„ProfIC Vario 15 Cation“ – Professional IC Vario system with Metrohm’s intelligent Partial Loop Injection Technique (MiPT)

The Professional IC Vario system with **Metrohm’s intelligent Partial Loop Injection Technique** and **conductivity detection** enables the fully automatic determination of cations or anions (non-suppressed). „Partial Loop Injection“ enables the injection of various sample volumes.

Typical areas of application:

- For universal application for all types of samples
- From trace analysis to waste water analysis
- Great differences in concentration in a single sample series

The „ProfIC Vario 15 Cation“ is comprised of one 940 Professional IC Vario ONE, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor, one 800 Dosino and the IC equipment for MiPT.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for

Technical Information

Parts

- 1 x 2.940.1100 940 Professional IC Vario ONE
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0010 858 Professional Sample Processor
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.180 IC equipment: MiPT


cooling and heating two iColumns and an external column position in the room temperature range.

The 800 Dosino and the IC equipment for MiPT enable Metrohm’s intelligent Partial Loop Injection Technique. 2 - 200 µL can be injected.

Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- MagIC Net

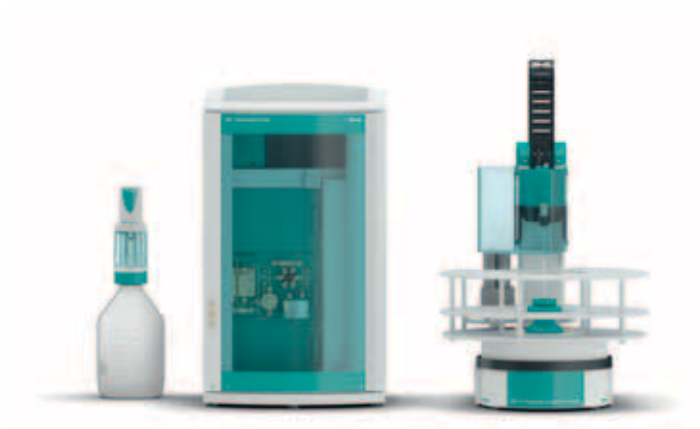

„ProfIC Vario 15 Cation“

Ordering Information

ProfIC Vario 15 Cation

„ProfIC Vario 1 Anion“ – Professional IC Vario system for automated ion chromatography

The Professional IC Vario system with **sequential suppression** and **conductivity detection** enables the fully automatic determination of anions.

Typical areas of application:

- Universally applicable anion analysis
- Routine analysis with large numbers of samples without additional sample preparation
- Coupling with MS or ICP/MS instruments for research and development tasks

The „ProfIC Vario 1 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector and one 858 Professional Sample Processor.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns, an external column position in the room tempera-

Technical Information

Parts

1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP

1 x 2.850.9010 IC Conductivity Detector

1 x 2.858.0020 858 Professional Sample Processor

ture range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.


The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 1 Anion

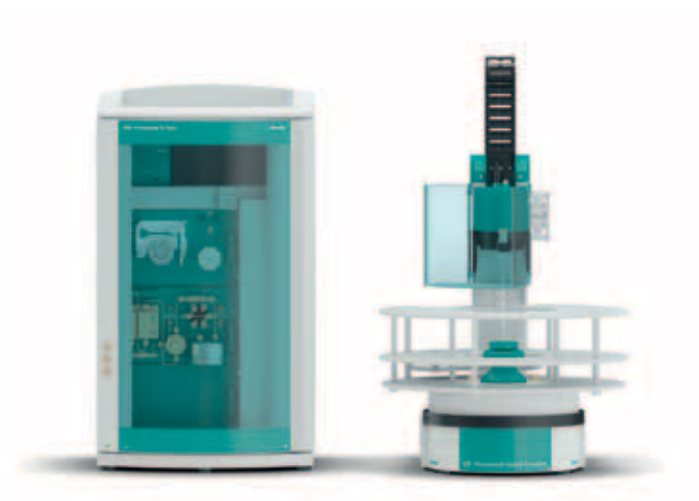

„ProfIC Vario 1 Anion“

„ProfIC Vario 1 Anion DR“ – Professional IC Vario system for automated ion chromatography with Dosino Regeneration of the suppressor

The Professional IC Vario system with **sequential suppression** with **Dosino Regeneration** of the suppressor and **conductivity detection** enables the fully automatic determination of anions.

Typical areas of application:

- Universally applicable anion analysis
- Routine analysis with large numbers of samples without additional sample preparation
- Coupling with MS or ICP/MS instruments for research and development tasks

The „ProfIC Vario 1 Anion DR“ is comprised of one 940 Professional IC Vario ONE/SeS, one „iDetector“ intelligent conductivity detector, one 800 Dosino, the 858 Professional Sample Processor and the IC equipment for Dosino Regeneration.

The 940 Professional IC Vario ONE/SeS is equipped with the „ONE“ and „SeS“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column

Technical Information

Parts

- 1 x 2.940.1400 940 Professional IC Vario ONE/SeS
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.190 IC equipment: Dosino Regeneration

thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application. The regeneration of the MSM is performed with one Dosino.


The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 1 Anion DR

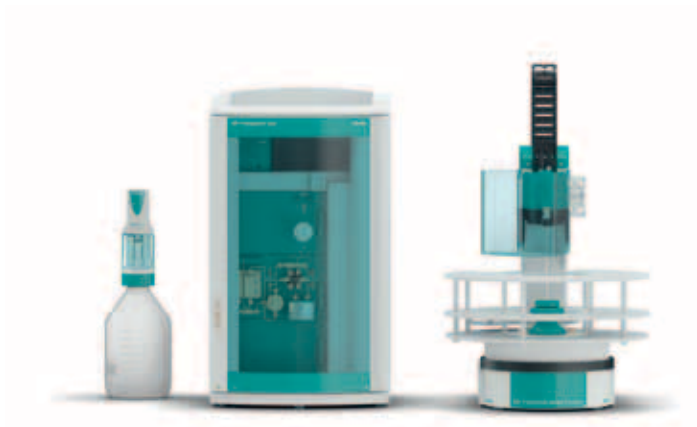


„ProfIC Vario 1 Anion DR“

Suppression repeatability

A fresh suppressor cartridge is used for each measurement with the „MSM“ Metrohm Suppressor Module. This ensures that one is always working with a cation exchanger that provides full performance: uninterrupted use today, tomorrow and for years into the future. The suppressor is distinguished by its pressure stability, it is 100% solvent-resistant and captivates by the length of its lifetime. Because no sensitive membranes are used, the suppressor achieves equilibrium and is ready for use in no time at all. It is only this way that a 10-year guarantee can be provided for the „MSM“.



The Metrohm Suppressor Module is inexpensive and robust. The fact that repeatability of the measurements with the „MSM“ is excellent is shown in the chromatograms:

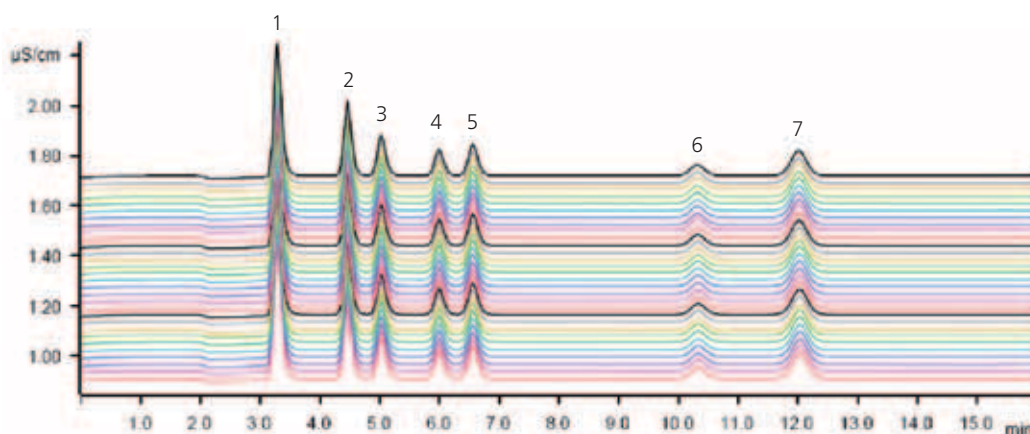

30 injections, separation of standard anions on the Metrosep A Supp 5 - 100/4.0, eluent 3.2 mmol/L Na_2CO_3 , 1.0 mmol/L NaHCO_3 , flow 0.7 mL/min, loop 20 μL , 45 °C, sequential suppression.

- 1 Fluoride
- 2 Chloride
- 3 Nitrite
- 4 Bromide
- 5 Nitrate
- 6 Phosphate
- 7 Sulfate

Ion	Fluoride	Chloride	Nitrite	Bromide	Nitrate	Phosphate	Sulfate
Concentration [mg/L]	0.25	0.25	0.25	0.25	0.25	0.25	0.25
Relative standard deviation in % (n = 30)	0.17	0.16	0.38	0.31	0.18	0.46	0.25

Sequential suppression

Sequential suppression is the chemical suppression combination using the „MSM, MSM-HC, MSM-LC“ with Metrohm CO₂ Suppression (MCS). This makes it possible to detect anions with carbonate/hydrogen carbonate eluents at the low background conductivity of hydroxide eluents.


The removal of CO₂ prevents the carbonate equilibrium from having a negative influence on the peak areas. The success: Up to 50% larger peak areas (and thus lower detection limits) result with the same concentration and the same sample volume. No carbonate peak also means no irritating interferences during the quantification of certain analyte anions. Chloride and carbonate coelute on many polystyrene-divinylbenzene columns, for example. This problem is now a thing of the past, thanks to the use of the CO₂ suppressor.

The extensive absence of the injection peak improves the determination of the rapidly eluting anions, e.g., of fluoride. Even though the separation of injection peak and fluoride peak is already very good on polyalcohol columns, the detection limit can be improved even more when the CO₂ suppressor is used. In addition, considerably larger sample volumes can be input, as there is practically no injection peak more to be seen.

No suppressor rotor or SPM rotor has been pre-installed. The rotors can be ordered individually in accordance with the respective application. The table shows the order numbers and the respective main application.

Suppressor rotor		
6.2832.000	MSM Rotor A	Suppressor rotor for standard applications
6.2842.000	MSM-HC Rotor A	Suppressor rotor for use with high-capacity columns or with long chromatogram duration
6.2844.000	MSM-LC Rotor A	Suppressor rotor for use with 2 mm separation columns
6.2835.000	SPM Rotor A	Rotor for inline sample preparation with cation exchange

Drinking water from Herisau (Switzerland): comparison of suppression with «MSM» (black) and with «MSM» plus «MCS» (red).

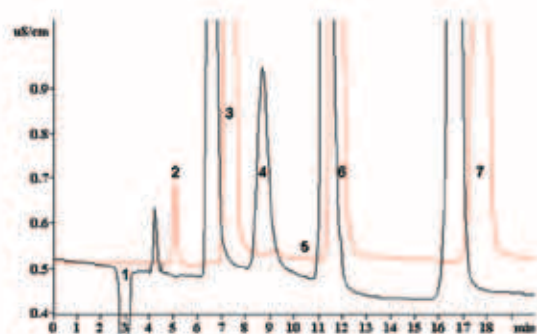

Column: Metrosep A Supp 5 - 100/4.0 (6.1006.510)
 Eluent: 3.2 mmol/L Na₂CO₃; 1.0 mmol/L NaHCO₃
 Flow rate: 0.4 mL/min

Nr.	Ion	Conz. (mg/L)
1	Injection peak	—
2	Fluoride	0.04
3	Chloride	7.79
4	Carbonate	
5	Bromide	0.004
6	Nitrate	7.82
7	Sulfate	5.20

„ProfIC Vario 2 Anion“ – Professional IC Vario system with Inline Ultrafiltration

The Professional IC Vario system with **Metrohm Inline Ultrafiltration** and **conductivity detection** enables the fully automatic determination of anions.

Typical areas of application:

- Samples with slight to medium-severe loads of particles, algae or bacteria
- Drinking and surface water
- Process and waste water

The „ProfIC Vario 2 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor and the IC equipment for Inline Ultrafiltration.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules.

The 940 Professional IC Vario ONE/SeS/PP can be used with or without chemical suppression. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive,

Technical Information

Parts

- 1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 6.5330.110 IC equipment: Inline Ultrafiltration

column thermostat for cooling and heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The IC equipment for Inline Ultrafiltration contains all of the parts needed for integrating Metrohm Inline Ultrafiltration in the system.


Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor. A minimum of 5 mL of sample is required for the Inline Ultrafiltration.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 2 Anion

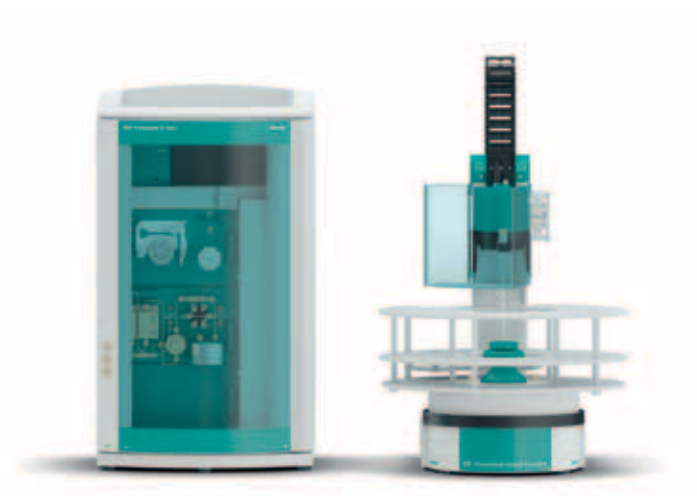

„ProfIC Vario 2 Anion“

„ProfIC Vario 3 Anion“ – Professional IC Vario system with Inline Dialysis

The Professional IC Vario system with **Metrohm Inline Dialysis** and **conductivity detection** enables the fully automatic determination of anions.

Typical areas of application:

- Samples with severe loads of particles, algae or bacteria
- Process, wash and waste water
- Emulsions, dispersions, cutting oils and samples containing petroleum
- Milk products and other samples containing protein

The „ProfIC Vario 3 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP/Prep 1, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor and one IC equipment for Inline Dialysis.

The 940 Professional IC Vario ONE/SeS/PP/Prep 1 is equipped with the „ONE“, „SeS/PP“ and „Prep 1“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and

Technical Information

Parts

- 1 x 2.940.1510 940 Prof. IC Vario ONE/SeS/PP/Prep 1
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 6.5330.100 IC equipment: Inline Dialysis

heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

In addition, a bidirectional two-channel peristaltic pump for sample preparation or sample injection is located in the lower segment of the instrument („Prep 1“). The position for the installation of the dialysis cell is prepared here.

The IC equipment for Inline Dialysis contains all of the parts required for the Metrohm-patented „Inline Stopped Flow Dialysis“.

Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor. At least 10 mL of sample are required for Inline Dialysis.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 3 Anion



„ProfIC Vario 3 Anion“



„ProfIC Vario 4 Anion“ – Professional IC Vario system with Inline Dilution

The Professional IC Vario system with **Metrohm's intelligent Inline Dilution** and **conductivity detection** enables the fully automatic determination of anions in concentrated solutions.

Typical areas of application:

- Samples with high ion concentration
- Samples from all industries

The „ProfIC Vario 4 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector, one 741 Magnetic Stirrer, one 800 Dosino and one IC equipment for Inline Dilution.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

Technical Information

Parts

- 1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 2.741.0010 741 Magnetic Stirrer
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.120 IC equipment: Inline Dilution

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The „ProfIC Vario 4 Anion“ offers the option of automatic inline dilution of every sample. This takes place at an external position on the 858 Professional Sample Processor. The 800 Dosino aspirates the volume to be diluted into the transfer tubing, doses it into the Liquid Handling Station and adds the required volume of dilution medium. All of the parts required are on hand with the IC equipment for Inline Dilution.

The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 4 Anion



„ProfIC Vario 4 Anion“

„ProfIC Vario 5 Anion“ – Professional IC Vario system with Metrohm’s intelligent preconcentration technique (MiPCT)

The Professional IC Vario system with **Metrohm’s intelligent inline sample preconcentration** and **conductivity detection** enables the fully automatic determination of anions in solutions with low ion concentration.

Typical areas of application:

- Numerous applications, ranging from ultrapure water analysis to drinking water analysis
- Analyses of different samples from power plants
- Process control and monitoring of rinsing solutions, e.g., in the semiconductor industry

The „ProfIC Vario 5 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector, one 800 Dosino, one 858 Professional Sample Processor and one IC equipment for MiPCT.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive,

Technical Information

Parts

- 1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0010 858 Professional Sample Processor
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.140 IC equipment: MiPCT

column thermostat for cooling and heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

With the 800 Dosino and the IC equipment for MiPCT, all of the parts required for Metrohm’s intelligent preconcentration technique are on hand.

The 858 Professional Sample Processor makes the samples available. The transfer takes place with the 800 Dosino. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 5 Anion



„ProfIC Vario 5 Anion“

„ProfIC Vario 6 Anion“ – Professional IC Vario system with Inline Dilution and Inline Ultrafiltration

The Professional IC Vario system with **Metrohm Inline Dilution**, **Metrohm Inline Ultrafiltration** and **conductivity detection** enables the fully automatic determination of anions that are present in very high concentrations and that have matrices containing particles.

Typical areas of application:

- Rinse, process and waste water
- Extractions and digestion solutions
- Food samples

The „ProfIC Vario 6 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector, one 741 Magnetic Stirrer, one 800 Dosino, one 858 Professional Sample Processor, an IC equipment for Inline Dilution and an IC equipment for Inline Ultrafiltration.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive,

Technical Information

Parts

- 1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 2.741.0010 741 Magnetic Stirrer
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.120 IC equipment: Inline Dilution
- 1 x 6.5330.110 IC equipment: Inline Ultrafiltration

column thermostat for cooling and heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump. The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The „ProfIC Vario 6 Anion“ offers the option of automatic inline dilution of every sample. This takes place at an external position on the 858 Professional Sample Processor. The 800 Dosino aspirates the volume to be diluted into the transfer tubing, doses it into the Liquid Handling Station and adds the required volume of dilution medium. All of the parts required are on hand with the IC equipment for Inline Dilution. The IC equipment for Inline Ultrafiltration contains all of the parts needed for integrating the subsequent Metrohm Inline Ultrafiltration in the system.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 6 Anion



„ProfIC Vario 6 Anion“

„ProfIC Vario 7 Anion“ – Professional IC Vario system with Inline Dilution and Inline Dialysis

The Professional IC Vario system with **Metrohm Inline Dilution, Inline Dialysis** and **conductivity detection** enables the fully automatic determination of anions that are present in high concentrations and in difficult matrices.

Typical areas of application:

- Process, wash and waste water
- Samples containing oil
- Inline Extraction for biodiesel analysis

The „ProfIC Vario 7 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP/Prep 1, one „iDetector“ intelligent conductivity detector, one 741 Magnetic Stirrer, one 800 Dosino, one 858 Professional Sample Processor, an IC equipment for Inline Dilution and an IC equipment for Inline Dialysis.

The 940 Professional IC Vario ONE/SeS/PP/Prep 1 is equipped with the „ONE“, „SeS/PP“ and „Prep 1“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with

Technical Information

Parts

1 x 2.940.1510	940 Prof. IC Vario ONE/SeS/PP/Prep 1
1 x 2.850.9010	IC Conductivity Detector
1 x 2.858.0020	858 Professional Sample Processor
1 x 2.741.0010	741 Magnetic Stirrer
1 x 2.800.0010	800 Dosino
1 x 6.5330.120	IC equipment: Inline Dilution
1 x 6.5330.100	IC equipment: Inline Dialysis

Maltese cross drive, column thermostat for cooling and heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump. The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The „ProfIC Vario 7 Anion“ offers the option of automatic inline dilution of every sample. This takes place at an external position on the 858 Professional Sample Processor. The 800 Dosino aspirates the volume to be diluted into the transfer tubing, doses it into the Liquid Handling Station and adds the required volume of dilution medium. All of the parts required are on hand with the IC equipment for Inline Dilution. The IC equipment for Inline Dialysis contains all of the parts required for the subsequent Metrohm-patented „Inline Stopped Flow Dialysis“.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 7 Anion



„ProfIC Vario 7 Anion“

„ProfIC Vario 8 Anion“ – Professional IC Vario system with Inline Matrix Elimination

The Professional IC Vario system with **Metrohm Inline Matrix Elimination** and **conductivity detection** enables the determination of anions in difficult matrices.

Typical areas of application:

- Trace analysis in polar solvents
- Quality controls in fuels, fuel mixtures and biofuels
- Quality management of chemicals

The „ProfIC Vario 8 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector and one 858 Professional Sample Processor.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

Technical Information

Parts

1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP
1 x 2.850.9010 IC Conductivity Detector
1 x 2.858.0030 858 Professional Sample Processor
1 x 6.1602.150 Bottle attachment / GL 45 - 3 x UNF
1 x 6.1608.070 Eluent bottle / 2 L / GL 45
1 x 6.1825.230 PEEK sample loop 10 µL

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.


The injector and the peristaltic pump on the 858 Professional Sample Processor and the additional accessory parts enable Inline Matrix Elimination. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor. As a rule, only small volumes with a maximum of 1 mL sample are required for matrix elimination.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 8 Anion

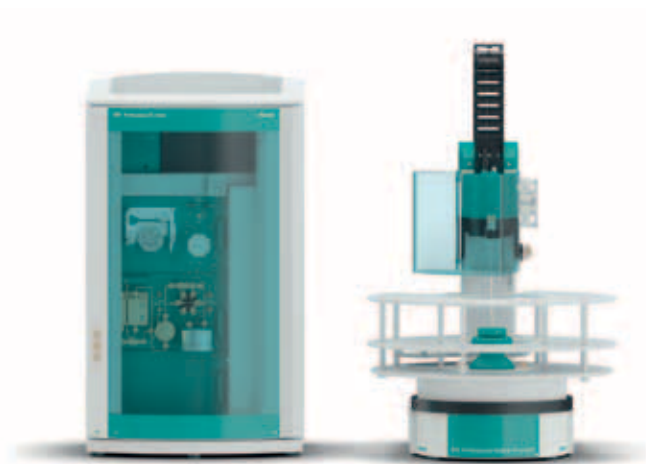

„ProfIC Vario 8 Anion“

„ProfIC Vario 9 Anion“ – Professional IC Vario system with Metrohm’s intelligent preconcentration technique and Inline Matrix Elimination (MiPCT-ME)

The Professional IC Vario system with **Metrohm’s intelligent inline preconcentration technique, Inline Matrix Elimination** and **conductivity detection** enables ultratrace analysis down to the lowest ppt range (ng/L) of anions in complex matrices.

Typical areas of application:

- Ultratrace analysis in samples from nuclear power plants and conventional power plants
- Trace and ultratrace analysis in extraction agents and organics
- Trace analysis in snow and ice

The „ProfIC Vario 9 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor, two 800 Dosinos and one IC equipment for MiPCT-ME.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation

Technical Information

Parts

- 1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0010 858 Professional Sample Processor
- 2 x 2.800.0010 800 Dosino
- 1 x 6.5330.160 IC equipment: MiPCT-ME

absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The two 800 Dosinos and the IC equipment for MiPCT-ME enable preconcentration of the sample and subsequent matrix elimination. Typical preconcentration volumes are 4 - 4,000 µL.

The 858 Professional Sample Processor makes the samples available. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 9 Anion



„ProfIC Vario 9 Anion“

„ProfIC Vario 10 Anion“ – Professional IC Vario system with Inline Neutralization

The Professional IC Vario system with **Metrohm Inline Neutralization** and **conductivity detection** enables the determination of anions in extremely alkali, acidic or metal-polluted matrices.

Typical areas of application:

- Trace analysis in bases and acids
- Starter substances from the electroplating industry
- Contaminations in electroplating baths

The „ProfIC Vario 10 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP/Prep 3, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor and additional accessory parts for In-line Neutralization.

The 940 Professional IC Vario ONE/SeS/PP/Prep 3 is equipped with the „ONE“, „SeS/PP“ and „Prep 3“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns, an external column position in

Technical Information

Parts

- 1 x 2.940.1530 940 Prof. IC Vario ONE/SeS/PP/Prep 3
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 6.2835.000 SPM Rotor A
- 1 x 2.858.0030 858 Professional Sample Processor
- 1 x 6.1602.150 Bottle attachment / GL 45 - 3 x UNF
- 1 x 6.1608.070 Eluent bottle / 2 L / GL 45
- 1 x 6.1825.230 PEEK sample loop 10 µL

the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.


In addition, the „SPM“ anion sample preparation module and a bidirectional two-channel peristaltic pump are located in the lower segment of the instrument („Prep 3“). Both of these components are used for Inline Neutralization and/or Inline Cation Removal. As a rule, only small volumes with a maximum of 1 mL sample are required for neutralization.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 10 Anion

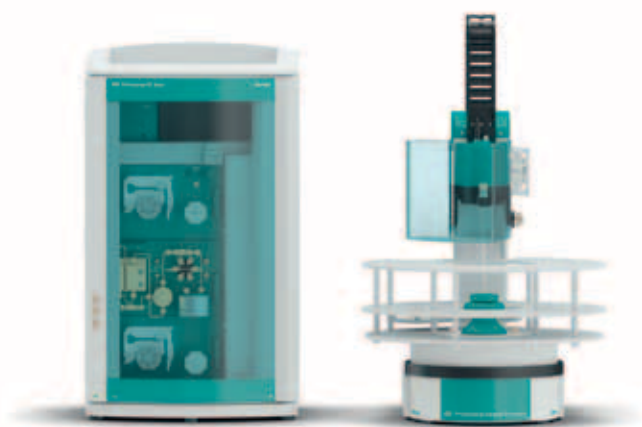

„ProfIC Vario 10 Anion“

„ProfIC Vario 11 Anion“ – Professional IC Vario system with Inline Neutralization, intelligent preconcentration technique and Inline Matrix Elimination

The Professional IC Vario system with **Metrohm Inline Neutralization, Metrohm's intelligent inline preconcentration technique, Inline Matrix Elimination** and **conductivity detection** enables the analysis of anions in complex matrices from the ultratrace down to the mg/L range.

Typical areas of application:

- Trace analysis in concentrated bases and acids
- Ultratrace analysis for nuclear power plants in matrices such as lithium hydroxide/boric acid

The „ProfIC Vario 11 Anion“ combines Inline Neutralization with MiPCT-ME. It is comprised of one 940 Professional IC Vario ONE/SeS/PP/Prep 3, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor, one 800 Dosino and the IC equipment for MiPCT.

The 940 Professional IC Vario ONE/SeS/PP/Prep 3 is equipped with the „ONE“, „SeS/PP“ and „Prep 3“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

Technical Information

Parts

- 1 x 2.940.1530 940 Prof. IC Vario ONE/SeS/PP/Prep 3
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0030 858 Professional Sample Processor
- 1 x 2.800.0010 800 Dosino
- 1 x 6.2832.000 MSM-A Rotor (for SPM)
- 1 x 6.2842.020 Adapter sleeve for Suppressor Vario
- 1 x 6.5330.140 IC equipment: MiPCT
- 1 x 6.1808.090 Thread adapter M8 outer / M6 inner
- 1 x 6.1014.200 Metrosep I Trap 1 - 100/4.0

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

In addition, the „SPM“ anion sample preparation module and a bidirectional two-channel peristaltic pump are located in the lower segment of the instrument („Prep 3“). Both components are used for the Metrohm Inline Neutralization.

The package contains the 800 Dosino and accessories for Metrohm's intelligent preconcentration technique. To accomplish this purpose, the 800 Dosino pumps the precise sample quantity through the SPM module to the preconcentration column and then removes the matrix afterwards with ultrapure water.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 11 Anion



„ProfIC Vario 11 Anion“

„ProfIC Vario 12 Anion“ – Professional IC Vario system for online monitoring, Metrohm’s intelligent preconcentration technique and Inline Matrix Elimination

The Professional IC Vario system with **selection valve** and **conductivity detection** enables **online** determination with **Metrohm’s intelligent preconcentration technique** and **matrix elimination** of anions from various sample flows.

Typical areas of application:

- Continuous analysis of processes
- Monitoring of drinking and surface water
- Monitoring of cooling water

The „ProfIC Vario 12 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector, one 942 Extension Module Vario LQH, one 800 Dosino and one IC equipment for MiPCT.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iCol-

Technical Information

Parts

- 1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.942.0070 942 Extension Module Vario LQH
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.140 IC equipment: MiPCT

umns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The 10-port valve contained in the 942 Extension Module LQH is used for selecting the various sample, standard and rinsing solutions.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- Suppressor rotor
- MagIC Net
- Communication between MagIC Net and the process control software

Ordering Information

ProfIC Vario 12 Anion



„ProfIC Vario 12 Anion“

„ProfIC Vario 14 Anion“ – Professional IC Vario system with Metrohm’s intelligent Pick-up-Injection Technique (MiPuT)

The Professional IC Vario system with **Metrohm’s intelligent Pick-up Injection Technique (MiPuT)** and **conductivity detection** enables the determination of anions from the smallest of sample volumes.

Typical areas of application:

- For universal application for all types of samples when only small sample quantities are available
- Investigation of biochemical processes
- Environmental sample extracts

The „ProfIC Vario 14 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor, one 800 Dosino and one IC equipment for MiPuT.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iCol-

Technical Information

Parts

- 1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP
- 1 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.170 IC equipment: MiPuT

umns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The 800 Dosino and the IC equipment for MiPuT enable Metrohm’s intelligent Pick-up Injection Technique. 2 - 50 µL of the samples can be removed and injected directly.

Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack (recommended 6.2041.480 Sample rack 159 x 2 mL + 3 x 300 mL)
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 14 Anion



„ProfIC Vario 14 Anion“

„ProfIC Vario 15 Anion“ – Professional IC Vario system with Metrohm’s intelligent Partial Loop Injection Technique (MiPT)

The Professional IC Vario system with **Metrohm’s intelligent Partial Loop Injection Technique** and **conductivity detection** enables the fully automated determination of anions. „Partial Loop Injection“ enables the injection of various sample volumes.

Typical areas of application:

- For universal application for all types of samples
- From trace analysis to waste water analysis
- Great differences in concentration in a single sample series

The „ProfIC Vario 15 Anion“ is comprised of one 940 Professional IC Vario ONE/SeS/PP, one „iDetector“ intelligent conductivity detector, one 858 Professional Sample Processor, one 800 Dosino and one IC equipment for MiPT.

The 940 Professional IC Vario ONE/SeS/PP is equipped with the „ONE“ and „SeS/PP“ modules. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive,

Technical Information

Parts

1 x 2.940.1500 940 Professional IC Vario ONE/SeS/PP

1 x 2.850.9010 IC Conductivity Detector

1 x 2.858.0010 858 Professional Sample Processor

1 x 2.800.0010 800 Dosino

1 x 6.5330.180 IC equipment: MiPT

column thermostat for cooling and heating two iColumns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with the drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The 800 Dosino and the IC equipment for MiPT enable Metrohm’s intelligent Partial Loop Injection Technique. 2 - 200 µL can be injected.

Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 15 Anion



„ProfIC Vario 15 Anion“

„ProfIC Vario 1 Amperometry“ – Professional IC Vario system for automated ion chromatography with amperometric detection

The Professional IC Vario system with **amperometric detection** enables the fully automatic determination of sugar, oxidizable anions and additional oxidizable and reducible components.

Typical areas of application:

- Universally applicable analysis of oxidizable or reducible components
- Routine analysis with large numbers of samples without additional sample preparation
- Sugar analysis with pulsed amperometric detection (PAD)
- Trace analysis of cyanide and sulfide with direct amperometric detection (DC)
- Analysis of additional oxidizable or reducible anions
- Determination of organic components with different potential forms (flexIPAD)

The „ProfIC Vario 1 Amperometry“ is comprised of one 940 Professional IC Vario ONE, one „iDetector“ intelligent amperometric detector and one 858 Professional Sample Processor.

Technical Information

Parts

- 1 x 2.940.1100 940 Professional IC Vario ONE
- 1 x 2.850.9110 IC Amperometric Detector
- 1 x 2.858.0020 858 Professional Sample Processor

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

The amperometric detector can be operated in four different modes (DC, PAD, flexIPAD and CV) and thus covers the entire application field of amperometric detection.


The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Amperometric measuring cell with the required electrodes
- Sample rack
- MagIC Net

Ordering Information

ProfIC Vario 1 Amperometry

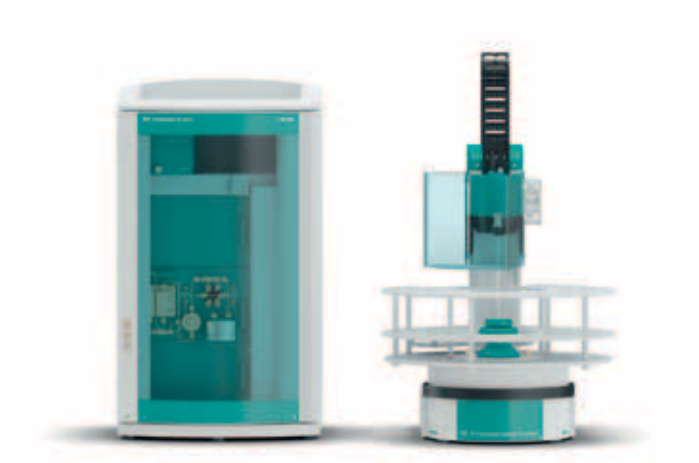

„ProfIC Vario 1 Amperometry“

„ProfIC Vario 1 UV/VIS“ – Professional IC Vario system for automated ion chromatography with UV/VIS detection

The Professional IC Vario system with **UV/VIS detection** enables the fully automated determination of anions, cations and organic compounds with optical absorption.

Typical areas of application:

- Universally applicable analysis for components that absorb UV or VIS light, respectively.
- Routine analysis with large numbers of samples without additional sample preparation

The „ProfIC Vario 1 UV/VIS“ is comprised of one 940 Professional IC Vario ONE, one 944 Professional UV/VIS Detector Vario and one 858 Professional Sample Processor.

The 940 Professional IC Vario ONE is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

Technical Information

Parts


- 1 x 2.940.1100 940 Professional IC Vario ONE
- 1 x 2.944.0010 944 Professional UV/VIS Detector Vario
- 1 x 2.858.0020 858 Professional Sample Processor

The 944 UV/VIS Detector Vario enables data acquisition at up to eight random wavelengths. In addition, the UV/VIS spectrum can be determined in the chromatogram at any time.

The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- MagIC Net

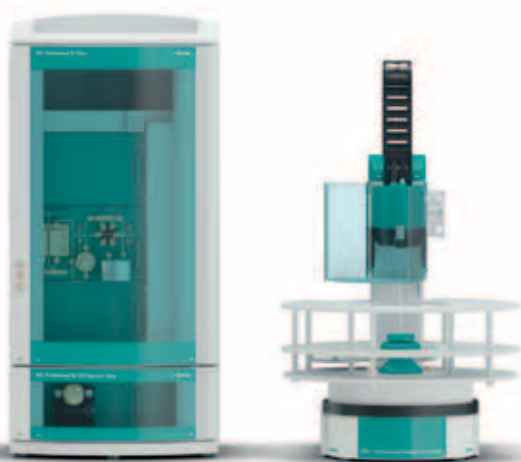

„ProfIC Vario 1 UV/VIS“

Ordering Information

ProfIC Vario 1 UV-VIS

„ProfIC Vario 1 PCR-UV/VIS“ – Professional IC Vario system for automated ion chromatography with post-column derivatization and UV/VIS detection

The Professional IC Vario system with **post-column derivatization** and **UV/VIS detection** enables the fully automated determination of anions, cations and additional components that can be converted using post-column derivatization into products with optical absorption.

Typical areas of application:

- Universal analysis with post-column derivatization and UV/VIS detection
- Analysis with large numbers of samples without additional sample preparation
- Trace analysis, e.g., of chromate, bromate, transition metals, etc.

The „ProfIC Vario 1 PCR-UV/VIS“ is comprised of one 940 Professional IC Vario ONE/Prep 1, one 944 Professional UV/VIS Detector Vario, one 943 Professional Reactor Vario and one 858 Professional Sample Processor.

The 940 Professional IC Vario ONE/Prep 1 is equipped with the „ONE“ module. It contains automatic sample and eluent degassing, „iPump“ IC high-pressure pump

Technical Information

Parts

1 x 2.940.1110	940 Professional IC Vario ONE/Prep 1
1 x 2.943.0110	943 Professional Reactor Vario
1 x 2.944.0010	944 Professional UV/VIS Detector Vario
1 x 2.858.0020	858 Professional Sample Processor
1 x 6.1608.030	Round glass bottle / 1,000 ml / GL 45
1 x 6.1602.150	Bottle attachment / GL 45 - 3 x UNF
1 x 6.1803.030	PTFE capillary 0.5 mm i.d. / 3 m

with intelligent pump head, pulsation absorber, six-way injection valve with Maltese cross drive, column thermostat for cooling and heating two iColumns and an external column position in the room temperature range.

In addition, a bidirectional two-channel peristaltic pump for conveying the post-column derivatization solution is located in the lower segment of the instrument („Prep 1“).

Post-column derivatization is performed in the 943 Professional Reactor Vario at temperatures up to 120 °C (or even up to 150 °C with the HT reactor plate).

The 944 Professional UV/VIS Detector Vario enables data acquisition at up to eight random wavelengths. In addition, the UV/VIS spectrum can be determined in the chromatogram at any time.

The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Sample rack
- MagIC Net

Ordering Information

ProfIC Vario 1 PCR-UV-VIS



„ProfIC Vario 1 PCR-UV/VIS“

„ProfIC Vario 1 AnCat“ – Professional IC Vario system for automated ion chromatography

The Professional IC Vario system with **conductivity detection** and **two analysis channels** enables the fully automatic determination of anions and cations, both in parallel and also completely independent from one another as a time-saving feature.

Typical areas of application:

- Universal anion and cation analysis
- Routine analysis with large numbers of samples without additional sample preparation

The „ProfIC Vario 1 AnCat“ is comprised of one 940 Professional IC Vario TWO/SeS/PP, two „iDetector“ intelligent conductivity detectors and one 858 Professional Sample Processor.

The 940 Professional IC Vario TWO/SeS/PP is equipped with two „ONE“ modules and one „SeS/PP“ module, thus resulting in an instrument with two analysis channels.

The instrument comprises automatic sample and eluent degassing for both channels, two „iPump“ IC high-pressure pumps with intelligent pump heads and pulsation

Technical Information

Parts

1 x 2.940.2500 940 Professional IC Vario TWO/SeS/PP

2 x 2.850.9010 IC Conductivity Detector

1 x 2.858.0020 858 Professional Sample Processor

absorbers, two six-way injection valves, a column thermostat for the cooling and heating of two „iColumn“ separation columns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with a drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.


The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation columns
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 1 AnCat

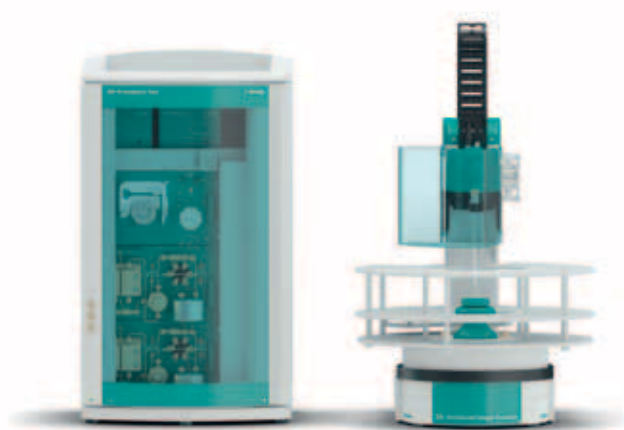

„ProfIC Vario 1 AnCat“

„ProfIC Vario 2 AnCat“ – Professional IC Vario system with Inline Ultrafiltration

The Professional IC Vario system with **Metrohm Inline Ultrafiltration** and **conductivity detection** enables the fully automatic determination of anions and cations.

Typical areas of application:

- Samples with slight to medium-severe loads of particles, algae or bacteria
- Drinking and surface water
- Process and waste water

The „ProfIC Vario 2 AnCat“ is comprised of one 940 Professional IC Vario TWO/SeS/PP, two intelligent conductivity detectors, one 858 Professional Sample Processor and an IC equipment for Inline Ultrafiltration.

The 940 Professional IC Vario TWO/SeS/PP is equipped with two „ONE“ modules and one „SeS/PP“ module, thus resulting in an instrument with two analysis channels.

The instrument comprises automatic sample and eluent degassing for both channels, two „iPump“ IC high-pressure pumps with intelligent pump heads and pulsation absorbers, two six-way injection valves, a column ther-

Technical Information

Parts

- 1 x 2.940.2500 940 Professional IC Vario TWO/SeS/PP
- 2 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 6.5330.110 IC equipment: Inline Ultrafiltration

mostat for the cooling and heating of two „iColumn“ separation columns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

It is equipped with a drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The IC equipment for Inline Ultrafiltration contains all of the parts needed for integrating Metrohm Inline Ultrafiltration in the system.


Numerous sample racks are available for volumes in the range of 0.5 - 500 mL for the 858 Professional Sample Processor. A minimum of 7 - 10 mL of sample is required for the Inline Ultrafiltration.

The following components must be ordered separately in accordance with the desired application:

- Separation columns
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 2 AnCat

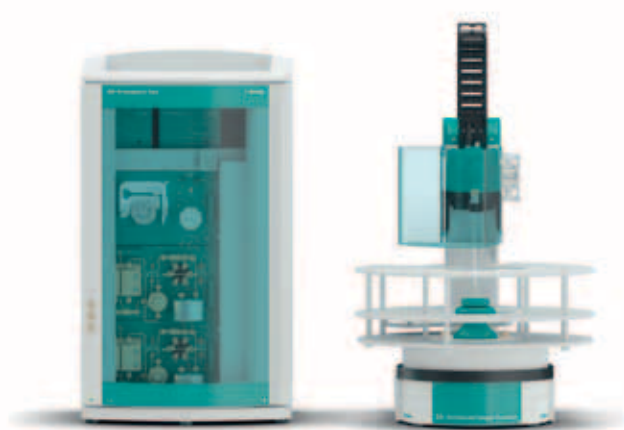

„ProfIC Vario 2 AnCat“

„ProfIC Vario 4 AnCat“ – Professional IC Vario system with Inline Dilution

The Professional IC Vario system with **Metrohm's intelligent Inline Dilution** and **conductivity detection** enables the fully automated determination of anions and cations in concentrated solutions.

Typical areas of application:

- Samples with high ion concentration
- Samples from all industries

The „ProfIC Vario 4 AnCat“ is comprised of one 940 Professional IC Vario TWO/SeS/PP, two „iDetector“ intelligent conductivity detectors, one 741 Magnetic Stirrer, one 800 Dosino and one IC equipment for Inline Dilution.

The 940 Professional IC Vario TWO/SeS/PP is equipped with two „ONE“ modules and one „SeS/PP“ module, thus resulting in an instrument with two analysis channels. It comprises automatic sample and eluent degassing for both channels, two „iPump“ IC high-pressure pumps with intelligent pump heads and pulsation absorbers, two six-way injection valves, a column thermostat for the cooling and heating of two „iColumn“ separation columns, an external column position in the room tem-

Technical Information

Parts

1 x 2.940.2500	940 Professional IC Vario TWO/SeS/PP
2 x 2.850.9010	IC Conductivity Detector
1 x 2.858.0020	858 Professional Sample Processor
1 x 2.741.0010	741 Magnetic Stirrer
1 x 2.800.0010	800 Dosino
1 x 6.5330.120	IC equipment: Inline Dilution

perature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with a drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.

The „ProfIC Vario 4 AnCat“ offers the option of automated inline dilution of every sample. This takes place at an external position on the 858 Professional Sample Processor. The 800 Dosino aspirates the volume to be diluted into the transfer tubing, doses it into the Liquid Handling Station and adds the required volume of dilution medium. All of the parts required are on hand with the IC equipment for Inline Dilution.


The 858 Professional Sample Processor takes care of the sample transfer. Numerous sample racks are available for volumes in the range of 0.5 - 500 mL.

The following components must be ordered separately in accordance with the desired application:

- Separation columns
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 4 AnCat

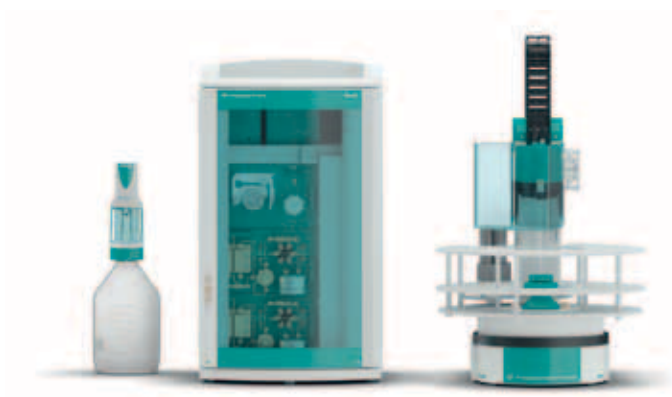

„ProfIC Vario 4 AnCat“

„ProfIC Vario 5 AnCat“ – Professional IC Vario system with Metrohm’s intelligent preconcentration technique (MiPCT)

The Professional IC Vario system with **Metrohm’s intelligent inline sample preconcentration** and **conductivity detection** enables the fully automatic determination of anions and cations in solutions with low ion concentration.

Typical areas of application:

- Numerous applications, ranging from ultrapure water analysis to drinking water analysis
- Analyses of different samples from power plants
- Process control and monitoring of rinsing solutions, e.g., in the semiconductor industry
- Trace analysis in snow and ice

The „ProfIC Vario 5 AnCat“ is comprised of one 940 Professional IC Vario TWO/SeS/PP, two „iDetector“ intelligent conductivity detectors, two 800 Dosinos, one 815 Robotic USB Sample Processor XL (2T/0P) with two workstations and two IC equipments for MiPCT.

The 940 Professional IC Vario TWO/SeS/PP is equipped with two „ONE“ modules and one „SeS/PP“ module, thus resulting in an instrument with two analysis channels.

Technical Information

Parts

- 1 x 2.940.2500 940 Professional IC Vario TWO/SeS/PP
- 2 x 2.850.9010 IC Conductivity Detector
- 1 x 2.815.0130 815 USB Sample Processor (2T/0P)
- 2 x 2.800.0010 800 Dosino
- 2 x 6.5330.140 IC equipment: MiPCT and additional parts for the Sample Processor

The instrument comprises automatic sample and eluent degassing for both channels, two „iPump“ IC high-pressure pumps with intelligent pump heads and pulsation absorbers, two six-way injection valves, a column thermostat for the cooling and heating of two „iColumn“ separation columns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump. The instrument is equipped with a drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted.

With the two 800 Dosinos and the two IC equipments for MiPCT, all of the parts required for Metrohm’s intelligent preconcentration technique in two-channel operation are on hand.

The two towers of the 814 USB Sample Processor (2T/0P) enable carry-over-free sampling for anion and cation determination through two independent sample needles.

The following components must be ordered separately in accordance with the desired application:

- Separation columns
- Preconcentration columns
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 5 AnCat



„ProfIC Vario 5 AnCat“

„ProfIC Vario 6 AnCat“ – Professional IC Vario system with Inline Dilution and Inline Ultrafiltration

The Professional IC Vario system with **Metrohm Inline Dilution**, **Metrohm Inline Ultrafiltration** and **conductivity detection** enables the fully automated determination of anions and cations that are present in very high concentrations and that have matrices containing particles.

Typical areas of application:

- Rinse, process and waste water
- Extractions and digestion solutions
- Food samples

The „ProfIC Vario 6 AnCat“ is comprised of one 940 Professional IC Vario TWO/SeS/PP, two „iDetector“ intelligent conductivity detectors, one 741 Magnetic Stirrer, one 800 Dosino, one 858 Professional Sample Processor, an IC equipment for Inline Dilution and an IC equipment for Inline Ultrafiltration.

The 940 Professional IC Vario TWO/SeS/PP is equipped with two „ONE“ modules and one „SeS/PP“ module, thus resulting in an instrument with two analysis channels. It comprises automatic sample and eluent degassing for

Technical Information

Parts

- 1 x 2.940.2500 940 Professional IC Vario TWO/SeS/PP
- 2 x 2.850.9010 IC Conductivity Detector
- 1 x 2.858.0020 858 Professional Sample Processor
- 1 x 2.741.0010 741 Magnetic Stirrer
- 1 x 2.800.0010 800 Dosino
- 1 x 6.5330.120 IC equipment: Inline Dilution
- 1 x 6.5330.110 IC equipment: Inline Ultrafiltration

both channels, two „iPump“ IC high-pressure pumps with intelligent pump heads and pulsation absorbers, two six-way injection valves, a column thermostat for the cooling and heating of two „iColumn“ separation columns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump. The instrument is equipped with a drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted.

The „ProfIC Vario 6 AnCat“ offers the option of automated inline dilution of every sample. This takes place at an external position on the 858 Professional Sample Processor. The 800 Dosino aspirates the volume to be diluted into the transfer tubing, doses it into the Liquid Handling Station and adds the required volume of dilution medium. With the IC equipment for Inline Dilution and for Inline Ultrafiltration, all of the parts needed to integrate Inline Dilution and Inline Ultrafiltration in the system are on hand.

The following components must be ordered separately in accordance with the desired application:

- Separation columns
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 6 AnCat



„ProfIC Vario 6 AnCat“

„ProfIC Vario 9 AnCat“ – Professional IC Vario system with Metrohm’s intelligent preconcentration technique and Inline Matrix Elimination (MiPCT-ME)

The Professional IC Vario system with **Metrohm’s intelligent inline preconcentration technique, Inline Matrix Elimination** and **conductivity detection** enables ultratrace analysis down to the lowest ppt range (ng/L) of anions and cations in complex matrices.

Typical areas of application:

- Ultratrace analysis in samples from nuclear power plants and conventional power plants
- Trace and ultratrace analysis in extraction agents and organics

The „ProfIC Vario 9 AnCat“ is comprised of one 940 Professional IC Vario TWO/SeS/PP, two „iDetector“ intelligent conductivity detectors, three 800 Dosinos, one 815 Robotic USB Sample Processor XL (2T/0P) with two workstations and one IC equipment each for MiPCT and MiPCT-ME.

The 940 Professional IC Vario TWO/SeS/PP is equipped with two „ONE“ modules and one „SeS/PP“ module, thus resulting in an instrument with two analysis channels. It comprises automatic sample and eluent degassing for

Technical Information

Parts

1 x 2.940.2500 940 Professional IC Vario TWO/SeS/PP
2 x 2.850.9010 IC Conductivity Detector
1 x 2.815.0130 815 USB Sample Processor (2T/0P)
3 x 2.800.0010 800 Dosino
1 x 6.5330.160 IC equipment: MiPCT-ME
1 x 6.5330.140 IC equipment: MiPCT
1 x 6.1014.200 Metrosep I Trap 1 - 100/4.0
and additional parts for the Sample Processor

both channels, two „iPump“ IC high-pressure pumps with intelligent pump heads and pulsation absorbers, two six-way injection valves, a column thermostat for the cooling and heating of two „iColumn“ separation columns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with a drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted.

One 800 Dosino each per sample channel and the IC equipments for MiPCT or MiPCT-ME, respectively, enable the preconcentration of the sample and the subsequent matrix elimination. Typical preconcentration volumes are 4 - 4,000 µL. The two towers of the 815 Robotic USB Sample Processor XL (2T/0P) enable carry-over-free sampling for anion and cation determination through two independent sample needles.

The following components must be ordered separately in accordance with the desired application:

- Separation column
- Preconcentration column
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 9 AnCat



„ProfIC Vario 9 AnCat“

„ProfIC Vario 14 AnCat“ – Professional IC Vario system with Metrohm’s intelligent Pick-up Injection Technique (MiPuT)

The Professional IC Vario system with **Metrohm’s intelligent Pick-up Injection Technique (MiPuT)** and **conductivity detection** enables the determination of anions and cations from the smallest of sample volumes.

Typical areas of application:

- For universal application for all types of samples when only small sample quantities are available
- Investigation of biochemical processes
- Environmental sample extracts

The „ProfIC Vario 14 AnCat“ is comprised of one 940 Professional IC Vario TWO/SeS/PP, two „iDetector“ intelligent conductivity detectors, one 858 Professional Sample Processor, one 800 Dosino and one IC equipment for MiPuT.

The 940 Professional IC Vario TWO/SeS/PP is equipped with two „ONE“ modules and one „SeS/PP“ module, thus resulting in an instrument with two analysis channels. It comprises automatic sample and eluent degassing for both channels, two „iPump“ IC high-pressure pumps with intelligent pump heads and pulsation absorbers,

Technical Information

Parts

1 x 2.940.2500	940 Professional IC Vario TWO/SeS/PP
2 x 2.850.9010	IC Conductivity Detector
1 x 2.858.0020	858 Professional Sample Processor
1 x 2.800.0010	800 Dosino
1 x 6.5330.170	IC equipment: MiPuT
1 x 6.1825.290	PEEK sample loop 250 µL

two six-way injection valves, a column thermostat for the cooling and heating of two „iColumn“ separation columns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with a drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.


The 800 Dosino and the IC equipment for MiPuT enable Metrohm’s intelligent Pick-up Injection Technique for both analysis channels. 2 - 50 µL of each of the samples can be removed and injected directly.

The following components must be ordered separately in accordance with the desired application:

- Separation columns
- Sample rack (recommended 6.2041.480 Sample rack 159 x 2 mL + 3 x 300 mL)
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 14 AnCat

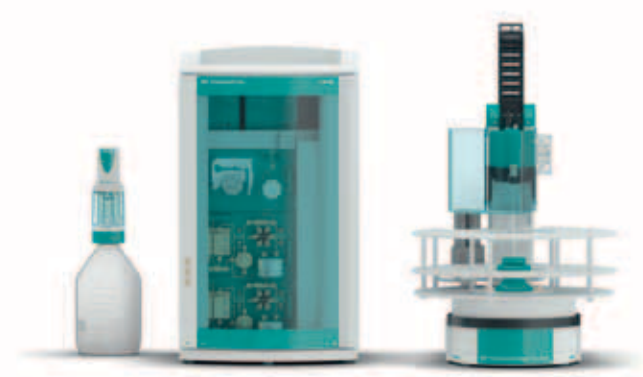

„ProfIC Vario 14 AnCat“

„ProfIC Vario 15 AnCat“ – Professional IC Vario system with Metrohm’s intelligent Partial Loop Injection Technique (MiPT)

The Professional IC Vario system with **Metrohm’s intelligent Partial Loop Injection Technique** and **conductivity detection** enables the fully automatic determination of anions and cations. „Partial Loop Injection“ enables the injection of various sample volumes.

Typical areas of application:

- For universal application for all types of samples
- From trace analysis to waste water analysis
- Great differences in concentration in a single sample series

The „ProfIC Vario 15 AnCat“ is comprised of one 940 Professional IC Vario TWO/SeS/PP, two „iDetector“ intelligent conductivity detectors, one 858 Professional Sample Processor, one 800 Dosino and the IC equipment for MiPT.

The 940 Professional IC Vario TWO/SeS/PP is equipped with two „ONE“ modules and one „SeS/PP“ module, thus resulting in an instrument with two analysis channels. It comprises automatic sample and eluent degassing for both channels, two „iPump“ IC high-pressure pumps

Technical Information

Parts

1 x 2.940.2500	940 Professional IC Vario TWO/SeS/PP
2 x 2.850.9010	IC Conductivity Detector
1 x 2.858.0010	858 Professional Sample Processor
1 x 2.800.0010	800 Dosino
1 x 6.5330.180	IC equipment: MiPT
1 x 6.1825.290	PEEK sample loop 250 µL
1 x 6.1841.000	PEEK transfer capillary 2 mL, 5 m
1 x 6.2744.080	M6 thread / UNF 10/32 coupling
1 x 6.2744.290	T connector 3 × UNF 10/32 with holder

with intelligent pump heads and pulsation absorbers, two six-way injection valves, a column thermostat for the cooling and heating of two „iColumn“ separation columns, an external column position in the room temperature range and a bidirectional two-channel peristaltic pump.

The instrument is equipped with a drive for the „MSM, MSM-HC and MSM-LC“ Metrohm Suppressor Module for chemical suppression and the „MCS“ Metrohm CO₂ Suppressor for CO₂ suppression. The combination of the two suppressors represents a sequential suppression and permits very sensitive analyses, thanks to the extremely low background conductivity. The suppressor rotor is not pre-mounted. This gives the customer different options to choose from and the suppressor rotor can be used in accordance with the respective application.


The 800 Dosino and the IC equipment for MiPT enable Metrohm’s intelligent Partial Loop Injection Technique. 2 - 200 µL can be injected.

The following components must be ordered separately in accordance with the desired application:

- Separation columns
- Sample rack
- Suppressor rotor
- MagIC Net

Ordering Information

ProfIC Vario 15 AnCat

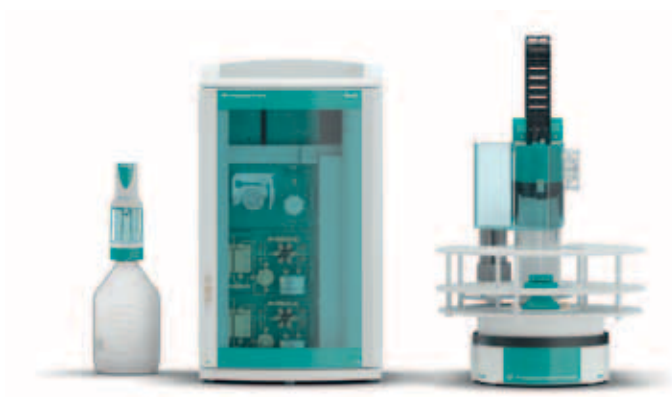

„ProfIC Vario 15 AnCat“

Professional IC Vario – Instruments

940 Professional IC Vario instruments – Introduction

940 Professional IC Vario – a system of innovative and intelligent components that are optimally coordinated with one another!

Configuration: The configuration of the system is as simple as possible, as the components log in automatically and make all relevant information available to the MagIC Net software.

Monitoring: The system monitors and optimizes all functions and documents them in accordance with FDA requirements upon request. Optimum operation of the 940 Professional IC Vario and the results are both monitored. If a parameter lies outside of the specified range, then the user will be informed via e-mail or SMS.

Inline Sample Preparation: The path from the sample to the precise result has become faster, as now even complex sample preparation steps are carried out inline and automatically. The system optimizes the sample preconcentration or the sample dilution automatically if required.

Free detector selection: The detection type can be selected to suit. That is the reason why no detector is included in the scope of delivery of the Professional IC Vario instruments.

- **Intelligent pump: iPump**
- **Intelligent detector: iDetector**
- **Intelligent column: iColumn**
- **Intelligent cells: iCell**
- **Intelligent reactors: iReactor**
- **Intelligent Liquid Handling with Dosinos**
- **Extension Module**

940 Professional IC Vario – Overview

		ONE	Suppression			Sample preparation			Gradient	
			Chemical	Sequential	MCS	Prep 1	Prep 2	Prep 3	HPG	LPG
		iPump + Inj.	MSM	MCS	PP	PP	PP + Inj.	PP + SPM		
2.940.1100	Professional IC Vario ONE	yes	–	–	–	–	–	–	–	–
2.940.1110	Professional IC Vario ONE/Prep 1	yes	–	–	–	yes	–	–	–	–
2.940.1120	Professional IC Vario ONE/Prep 2	yes	–	–	–	–	yes	–	–	–
2.940.1140	Professional IC Vario ONE/HPG	yes	–	–	–	–	–	–	yes	–
2.940.1150	Professional IC Vario ONE/LPG	yes	–	–	–	–	–	–	–	yes
2.940.1200	Professional IC Vario ONE/ChS	yes	yes	–	–	–	–	–	–	–
2.940.1240	Professional IC Vario ONE/ChS/HPG	yes	yes	–	–	–	–	–	–	–
2.940.1250	Professional IC Vario ONE/ChS/LPG	yes	yes	–	–	–	–	–	–	–
2.940.1300	Professional IC Vario ONE/ChS/PP	yes	yes	–	yes	–	–	–	–	–
2.940.1340	Professional IC Vario ONE/ChS/PP/HPG	yes	yes	–	yes	–	–	–	yes	–
2.940.1350	Professional IC Vario ONE/ChS/PP/LPG	yes	yes	–	yes	–	–	–	–	yes
2.940.1400	Professional IC Vario SeS	yes	yes	yes	–	–	–	–	–	–
2.940.1410	Professional IC Vario SeS/Prep 1	yes	yes	yes	–	yes	–	–	–	–
2.940.1420	Professional IC Vario SeS/Prep 2	yes	yes	yes	–	–	yes	–	–	–
2.940.1430	Professional IC Vario SeS/Prep 3	yes	yes	yes	–	–	–	yes	–	–
2.940.1440	Professional IC Vario SeS/HPG	yes	yes	yes	–	–	–	–	yes	–
2.940.1450	Professional IC Vario SeS/LPG	yes	yes	yes	–	–	–	–	–	yes
2.940.1500	Professional IC Vario SeS/PP	yes	yes	yes	yes	–	–	–	–	–
2.940.1510	Professional IC Vario SeS/PP/Prep 1	yes	yes	yes	yes	yes	–	–	–	–
2.940.1520	Professional IC Vario SeS/PP/Prep 2	yes	yes	yes	yes	–	yes	–	–	–
2.940.1530	Professional IC Vario SeS/PP/Prep 3	yes	yes	yes	yes	–	–	yes	–	–
2.940.1540	Professional IC Vario SeS/PP/HPG	yes	yes	yes	yes	–	–	–	yes	–
2.940.1550	Professional IC Vario SeS/PP/LPG	yes	yes	yes	yes	–	–	–	–	yes
2.940.2100	Professional IC Vario TWO	yes (2x)	–	–	–	–	–	–	–	–
2.940.2200	Professional IC Vario TWO/ChS	yes (2x)	yes	–	–	–	–	–	–	–
2.940.2300	Professional IC Vario TWO/ChS/PP	yes (2x)	yes	–	yes	–	–	–	–	–
2.940.2400	Professional IC Vario TWO/SeS	yes (2x)	yes	yes	–	–	–	–	–	–
2.940.2500	Professional IC Vario TWO/SeS/PP	yes (2x)	yes	yes	yes	–	–	–	–	–

Professional IC Vario instruments

940 Professional IC Vario ONE (2.940.1100)

The 940 Professional IC Vario ONE is the intelligent IC instrument for applications **without suppression**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/Prep 1 (2.940.1110)

The 940 Professional IC Vario ONE/Prep 1 is the intelligent IC instrument **without suppression** in combination with Metrohm Inline Sample Preparation, e.g., **In-line Ultrafiltration** or **In-line Dialysis**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/Prep 2 (2.940.1120)

The 940 Professional IC Vario ONE/Prep 2 is the intelligent IC instrument **without suppression** in combination with Metrohm Inline Sample Preparation, e.g., **In-line Matrix Elimination** or **In-line Calibration**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/HPG (2.940.1140)

The 940 Professional IC Vario ONE/HPG is the intelligent IC instrument **without suppression** with **binary high-pressure gradient**. It can be extended with the 942 Extension Modules to up to a quaternary gradient system. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/LPG (2.940.1150)

The 940 Professional IC Vario ONE/LPG is the intelligent IC instrument **without suppression** with **low-pressure gradient**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/ChS (2.940.1200)

The 940 Professional IC Vario ONE/ChS is the intelligent IC instrument with **chemical suppression**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/ChS/HPG (2.940.1240)

The 940 Professional IC Vario ONE/ChS/HPG is the intelligent IC instrument with **chemical suppression** and **binary high-pressure gradient**. It can be extended with the 942 Extension Modules to up to a quaternary gradient system. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/ChS/LPG (2.940.1250)

The 940 Professional IC Vario ONE/ChS/LPG is the intelligent IC instrument with **chemical suppression** and **low-pressure gradient**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/ChS/PP (2.940.1300)

The 940 Professional IC Vario ONE/ChS/PP is the intelligent IC instrument with **chemical suppression** and a **peristaltic pump** for suppressor regeneration. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/ChS/PP/HPG (2.940.1340)

The 940 Professional IC Vario ONE/ChS/PP/HPG is the intelligent IC instrument with **chemical suppression**, a **peristaltic pump** for suppressor regeneration and **binary high-pressure gradient**. It can be extended with the 942 Extension Modules to up to a quaternary gradient system. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/ChS/PP/LPG (2.940.1350)

The 940 Professional IC Vario ONE/ChS/PP/LPG is the intelligent IC instrument with **chemical suppression**, a **peristaltic pump** for suppressor regeneration and **low-pressure gradient**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS (2.940.1400)

The 940 Professional IC Vario ONE/SeS is the intelligent IC instrument for applications with **sequential suppression**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/Prep 1
(2.940.1410)

The 940 Professional IC Vario ONE/SeS/Prep 1 is the intelligent IC instrument with **sequential suppression** in combination with Metrohm Inline Sample Preparation, e.g., **Inline Ultrafiltration** or **Inline Dialysis**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/Prep 2
(2.940.1420)

The 940 Professional IC Vario ONE/SeS/Prep 2 is the intelligent IC instrument with **sequential suppression** in combination with Metrohm Inline Sample Preparation, e.g., **Inline Matrix Elimination** or **Inline Calibration**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/Prep 3
(2.940.1430)

The 940 Professional IC Vario ONE/SeS/Prep 3 is the intelligent IC instrument with **sequential suppression** in combination with Metrohm Inline Sample Preparation, e.g., **Inline Neutralization** or **Inline Cation Removal**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/HPG (2.940.1440)

The 940 Professional IC Vario ONE/SeS/HPG is the intelligent IC instrument with **sequential suppression** and **binary high-pressure gradient**. It can be extended with the 942 Extension Modules to up to a quaternary gradient system. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/LPG (2.940.1450)

The 940 Professional IC Vario ONE/SeS/LPG is the intelligent IC instrument with **sequential suppression** and **low-pressure gradient**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/PP (2.940.1500)

The 940 Professional IC Vario ONE/SeS/PP is the intelligent IC instrument with **sequential suppression** and a **peristaltic pump** for suppressor regeneration. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/PP/Prep 1 (2.940.1510)

The 940 Professional IC Vario ONE/SeS/PP/Prep 1 is the intelligent IC instrument with **sequential suppression** and a **peristaltic pump** for suppressor regeneration in combination with Metrohm Inline Sample Preparation, e.g., **Inline Ultrafiltration** or **Inline Dialysis**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/PP/Prep 2 (2.940.1520)

The 940 Professional IC Vario ONE/SeS/PP/Prep 2 is the intelligent IC instrument with **sequential suppression** and a **peristaltic pump** for suppressor regeneration in combination with Metrohm Inline Sample Preparation, e.g., **Inline Matrix Elimination** or **Inline Calibration**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/PP/Prep 3
(2.940.1530)

The 940 Professional IC Vario ONE/SeS/PP/Prep 3 is the intelligent IC instrument with **sequential suppression** with a **peristaltic pump** for suppressor regeneration in combination with Metrohm Inline Sample Preparation, e.g., **Inline Neutralization** or **Inline Cation Removal**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/PP/HPG
(2.940.1540)

The 940 Professional IC Vario ONE/SeS/PP/HPG is the intelligent IC instrument with **sequential suppression**, a **peristaltic pump** for suppressor regeneration and **binary high-pressure gradient**. It can be extended with the 942 Extension Modules to up to a quaternary gradient system. The instrument can be used with any separation and detection methods.



940 Professional IC Vario ONE/SeS/PP/LPG
(2.940.1550)

The 940 Professional IC Vario ONE/SeS/PP/LPG is the intelligent IC instrument with **sequential suppression**, a **peristaltic pump** for suppressor regeneration and **low-pressure gradient**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario TWO (2.940.2100)

The 940 Professional IC Vario TWO is the intelligent **two-channel** IC instrument **without suppression**. The instrument can be used with any separation and detection methods.



940 Professional IC Vario TWO/ChS (2.940.2200)

The 940 Professional IC Vario TWO/ChS is the intelligent **two-channel** IC instrument with a **chemical suppressor**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario TWO/ChS/PP (2.940.2300)

The 940 Professional IC Vario TWO/ChS/PP is the intelligent **two-channel** IC instrument with a **chemical suppressor** and a **peristaltic pump** for suppressor regeneration. The instrument can be used with any separation and detection methods.



940 Professional IC Vario TWO/SeS (2.940.2400)

The 940 Professional IC Vario TWO/SeS is the intelligent **two-channel** IC instrument with **sequential suppression** (one channel). An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



940 Professional IC Vario TWO/SeS/PP (2.940.2500)

The 940 Professional IC Vario TWO/SeS/PP is the intelligent **two-channel** IC instrument with **sequential suppression** (one channel) and a **peristaltic pump** for suppressor regeneration. The instrument can be used with any separation and detection methods.



Professional IC Vario – Detectors


IC Conductivity Detector (2.850.9010)

Compact and intelligent high performance conductivity detector for intelligent IC instruments. Outstanding temperature stability, the complete signal processing within the protected detector block and the latest generation of DSP – Digital Signal Processing – guarantee the highest precision of the measurement. No change of measuring ranges (not even automatic ones) is required, due to the dynamic working range.




IC Amperometric Detector (2.850.9110)

Compact and intelligent amperometric detector for intelligent IC instruments. Outstanding selectivity due to the four measuring modes: DC, PAD, flexIPAD and CV, as well as the excellent signal/noise ratio and the very fast stabilization of the measuring signal guarantee the highest in measurement precision.

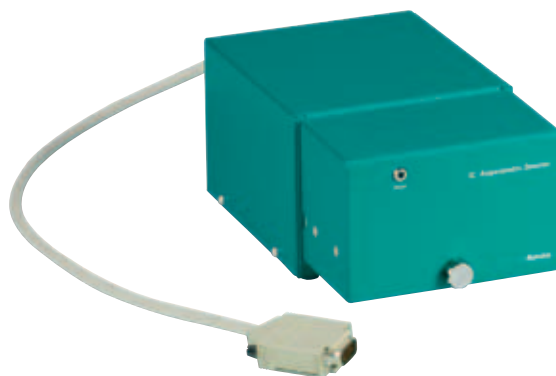

944 Professional UV/VIS Detector Vario (2.944.0010)

The 944 Professional UV/VIS Detector Vario is the intelligent UV/VIS detector from Metrohm. It permits a secure and reliable quantification of substances active in the ultraviolet or visible range. Detection takes place via a Diode Array.

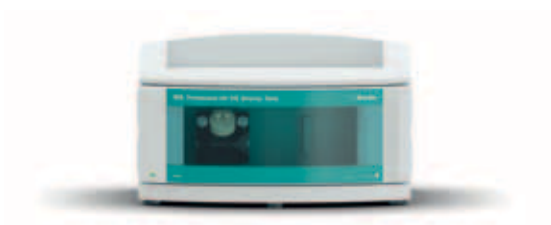


945 Professional Detector Vario – Conductivity (2.945.0010)

Intelligent stand-alone detector equipped with a high-performance IC Conductivity Detector. For use with intelligent IC instruments or as independent conductivity detector.



945 Professional Detector Vario – Amperometry
(2.945.0020)

Intelligent stand-alone detector equipped with the IC Amperometric Detector. Outstanding selectivity due to the four measuring modes: DC, PAD, flexIPAD, CV. The excellent signal/noise ratio and the very fast start-up guarantee the highest in measurement precision. For use with intelligent IC instruments or as independent detector.

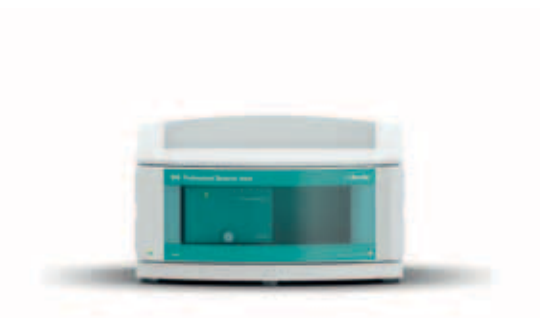

945 Professional Detector Vario – Conductivity & Amperometry
(2.945.0030)

Intelligent stand-alone detector equipped with the high performance IC Conductivity Detector and the IC Amperometric Detector, with the four measuring modes DC, PAD, flexIPAD and CV. For use with intelligent IC instruments or as independent detector for conductivity and amperometric detection.



Inline Eluent Preparation – Introduction

Inline Eluent Preparation

Inline Eluent Preparation increases the duration of unattended operation in that with this system, the exhausted eluent is refilled fully automatically while the ion chromatograph is in operation. The eluent is diluted in portions with ultrapure water from an eluent concentrate for this purpose.

For automatic Inline Eluent Preparation, the 940 Professional IC Vario intelligent ion chromatography systems or the instruments in the Compact IC line need only be expanded to include a 941 Eluent Production Module. While the latter monitors the eluent fill level, the 800 Dosino is responsible for all dosing and Liquid Handling tasks.

Tests with injections of 250 µg/L standard solutions, spread out over a time period of approximately 20 days, have demonstrated outstanding stability with respect to retention times. After more than 800 sample injections, the relative standard deviations for a series of anions and cations were less than 0.55 and 0.41 percent, respectively. During a test sequence over a 24-hour period, the precision of the retention times for anions and cations were better than 0.09 and 0.08 percent, respectively. In short, Inline Eluent Preparation with the 941 Eluent Production Module increases the reproducibility of retention times, thus permitting the exact analysis of anions and cations over extended periods, and does so without manual eluent production.


941 Eluent Production Module

The 941 Eluent Production Module enables the automatic production of an eluent. It enables continuous working without manual intervention and guarantees stable retention times. It can be combined with all Metrohm IC instruments and is monitored by MagIC Net.

The 941 Eluent Production Module is equipped for the production of an eluent and contains an 800 Dosino. Additional eluents can be produced and monitored when it is expanded to include an 800 Dosino with the IC equipment for additional eluents (6.5330.090).

In addition, it offers the possibility of directly connecting an ultrapure water system (ELGA PURELAB® flex 5 or flex 6).

- „Inline Eluent Preparation“
- Enhances laboratory safety
- Protects eluents against idle running
- Can be used for all types of eluents
- Simple assembly and configuration
- Guarantees stable retention times
- Uninterrupted working without manual intervention

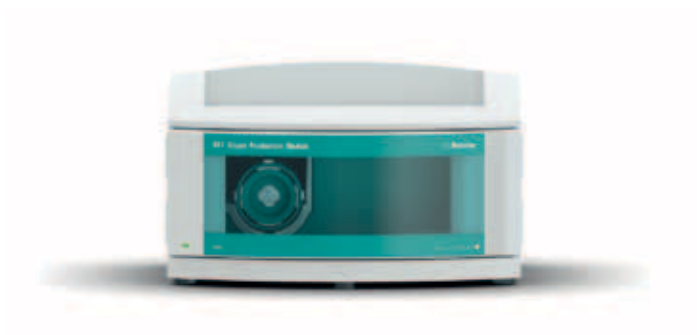

941 Eluent Production Module

Ordering Information

2.941.0010 941 Eluent Production Module

Extension Module Vario – Overview

		ONE	LQH	Suppression			Sample preparation		Gradient
		iPump + Injector	PP + Inj. + Selector	chemical	sequential		Prep 2	Prep 3	HPG
				MSM	MCS	PP	PP + Inj.	PP + SPM	
2.942.0020	Extension Module Vario Prep 2	–	–	–	–	–	yes	–	–
2.942.0040	Extension Module Vario HPG	–	–	–	–	–	–	–	yes
2.942.0070	Extension Module Vario LQH	–	yes	–	–	–	–	–	–
2.942.0300	Extension Module Vario ChS/PP	–	–	yes	–	yes	–	yes	–
2.942.0500	Extension Module Vario SeS/PP	–	–	yes	yes	yes	–	–	–
2.942.1060	Extension Module Vario ONE/Deg	yes	–	–	–	–	–	–	–



Extension Module Vario

942 Extension Module Vario Prep 2 (2.942.0020)

The 942 Extension Module Vario Prep 2 is an extension module for the Professional IC Vario line of instruments. It multiplies the possibilities of **Inline Sample Preparation** and **Liquid Handling** in Professional IC Vario systems.



942 Extension Module Vario HPG (2.942.0040)

The 942 Extension Module Vario HPG is an extension module for the Professional IC Vario line of instruments. It permits the addition of a further eluent in a Professional IC Vario **high-pressure gradient system**.



942 Extension Module Vario LQH (2.942.0070)

The 942 Extension Module Vario LQH is an extension module for the Professional IC Vario line of instruments. It expands the possibilities of **Metrohm Inline Sample Preparation „MISP“** and **Liquid Handling** and opens a Professional IC system for **Online Monitoring**.



942 Extension Module Vario ChS/PP (2.942.0300)

The 942 Extension Module Vario ChS/PP is an extension module for the Professional IC Vario line of instruments. It permits the integration of a complete **chemical suppression** with a **peristaltic pump** for suppressor regeneration or **Inline Neutralization** or **Inline Cation Removal**, respectively, in a Professional IC Vario system.



942 Extension Module Vario SeS/PP (2.942.0500)

The 942 Extension Module Vario SeS/PP is an extension module for the Professional IC Vario line of instruments. It permits the integration of a complete **sequential suppression** with **peristaltic pump** for suppressor regeneration in a Professional IC Vario system.



942 Extension Module Vario ONE/Deg (2.942.1060)

The 942 Extension Module Vario ONE/Deg is an extension module for the Professional IC Vario line of instruments. It permits the installation of an additional **IC analysis channel** in a Professional IC Vario system.



Compact IC Flex – Instruments

Compact IC Flex – Introduction

The intelligent instrument generation of the Compact ion chromatographs

930 Compact IC Flex and 883 Basic IC plus

Intelligent. Safe. Precise.

The top model for ion chromatography from Metrohm is the 940 Professional IC Vario. Its intelligent system components set standards with respect to the precision of the results and operating convenience. This technology is also available in the intelligent generation of the Compact line of instruments. The 930 Compact IC Flex is oriented to users from all industries that have a defined need for analysis. Determination of anions, cations and polar substances in the $\mu\text{g/L}$ to g/L range is accurate and securely possible.

All intelligent functions of the Professional IC Vario instrument series are also integrated in the 940 Compact Flex and 883 Basic instruments: iPump, iDetector, iColumn technology. They guarantee precise results and exclude the possibility of operator errors to a maximum extent. The MagIC Net chromatography software con-

trols all system components and permits the monitoring of all relevant parameters.

Depending on the version selected, the 930 Compact IC Flex instruments are equipped with chemical or sequential suppression, one column oven and eluent and sample degassers. The type of detection can be selected to suit. That is the reason why no detector is included in the scope of delivery of the Compact IC instruments.

The 883 Basic IC plus is the optimum instrument for training purposes. It can be operated only with the supplied IC Conductivity Detector.

Access to the new online configurator for the 930 Compact IC Flex instruments is through ic930.metrohm.com



Compact IC Flex – Overview

		Suppression			Column oven	Degasser	Automation capability	863 Autosampler included	Software included
		chemical	sequential						
		MSM	MCS	PP					
2.930.1100	Compact IC Flex	–	–	–	–	–	yes	–	–
2.930.1160	Compact IC Flex Deg	–	–	–	–	yes	yes	–	–
2.930.1200	Compact IC Flex ChS	yes	–	–	–	–	yes	–	–
2.930.1260	Compact IC Flex ChS/Deg	yes	–	–	–	yes	yes	–	–
2.930.1300	Compact IC Flex ChS/PP	yes	–	yes	–	–	yes	–	–
2.930.1360	Compact IC Flex ChS/PP/Deg	yes	–	yes	–	yes	yes	–	–
2.930.1400	Compact IC Flex SeS	yes	yes	–	–	–	yes	–	–
2.930.1460	Compact IC Flex SeS/Deg	yes	yes	–	–	yes	yes	–	–
2.930.1500	Compact IC Flex SeS/PP	yes	yes	yes	–	–	yes	–	–
2.930.1560	Compact IC Flex SeS/PP/Deg	yes	yes	yes	–	yes	yes	–	–
2.930.2100	Compact IC Flex Oven	–	–	–	yes	–	yes	–	–
2.930.2160	Compact IC Flex Oven/Deg	–	–	–	yes	yes	yes	–	–
2.930.2200	Compact IC Flex Oven/ChS	yes	–	–	yes	–	yes	–	–
2.930.2260	Compact IC Flex Oven/ChS/Deg	yes	–	–	yes	yes	yes	–	–
2.930.2300	Compact IC Flex Oven/ChS/PP	yes	–	yes	yes	–	yes	–	–
2.930.2360	Compact IC Flex Oven/ChS/PP/Deg	yes	–	yes	yes	yes	yes	–	–
2.930.2400	Compact IC Flex Oven/SeS	yes	yes	–	yes	–	yes	–	–
2.930.2460	Compact IC Flex Oven/SeS/Deg	yes	yes	–	yes	yes	yes	–	–
2.930.2500	Compact IC Flex Oven/SeS/PP	yes	yes	yes	yes	–	yes	–	–
2.930.2560	Compact IC Flex Oven/SeS/PP/Deg	yes	yes	yes	yes	yes	yes	–	–
2.883.0020	Basic IC plus	yes	–	yes	–	–	yes	–	yes
2.883.1020	Basic IC plus Package	yes	–	yes	–	–	yes	yes	yes

Compact IC Flex

930 Compact IC Flex (2.930.1100)

The 930 Compact IC Flex is the intelligent Compact IC instrument **without suppression**. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Deg (2.930.1160)

The 930 Compact IC Flex Deg is the intelligent Compact IC instrument **without suppression** with built-in **degasser**. The instrument can be used with any separation and detection methods.



930 Compact IC Flex ChS (2.930.1200)

The 930 Compact IC Flex ChS is the intelligent Compact IC instrument with **chemical suppression**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



930 Compact IC Flex ChS/Deg (2.930.1260)

The 930 Compact IC Flex ChS/Deg is the intelligent Compact IC instrument with **chemical suppression** and built-in **degasser**. An 800 Dosino is used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



930 Compact IC Flex ChS/PP (2.930.1300)

The 930 Compact IC Flex ChS/PP is the intelligent Compact IC instrument with **chemical suppression** and a **peristaltic pump** for regeneration. The instrument can be used with any separation and detection methods.



930 Compact IC Flex ChS/PP/Deg (2.930.1360)

The 930 Compact IC Flex ChS/PP/Deg is the intelligent Compact IC instrument with **chemical suppression** and a **peristaltic pump** for regeneration and a built-in **degasser**. The instrument can be used with any separation and detection methods.



930 Compact IC Flex SeS (2.930.1400)

The 930 Compact IC Flex SeS is the intelligent Compact IC instrument with **sequential suppression**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



930 Compact IC Flex SeS/Deg (2.930.1460)

The 930 Compact IC Flex SeS/Deg is the intelligent Compact IC instrument with **sequential suppression** and built-in **degasser**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



930 Compact IC Flex SeS/PP (2.930.1500)

The 930 Compact IC Flex SeS/PP is the intelligent Compact IC instrument with **sequential suppression** and a **peristaltic pump** for suppressor regeneration. The instrument can be used with any separation and detection methods.



930 Compact IC Flex SeS/PP/Deg (2.930.1560)

The 930 Compact IC Flex SeS/PP/Deg is the intelligent Compact IC instrument with **sequential suppression** and a **peristaltic pump** for suppressor regeneration, in addition to a built-in **degasser**. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven (2.930.2100)

The 930 Compact IC Flex Oven is the intelligent Compact IC instrument with **column oven** and **without suppression**. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven/Deg (2.930.2160)

The 930 Compact IC Flex Oven/Deg is the intelligent Compact IC instrument with **column oven, without suppression** and with built-in **degasser**. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven/ChS (2.930.2200)

The 930 Compact IC Flex Oven/ChS is the intelligent Compact IC instrument with **column oven** and **chemical suppression**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven/ChS/Deg (2.930.2260)

The 930 Compact IC Flex Oven/ChS/Deg is the intelligent Compact IC instrument with **column oven**, **chemical suppression** and built-in **degasser**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven/ChS/PP (2.930.2300)

The 930 Compact IC Flex Oven/ChS/PP is the intelligent Compact IC instrument with **column oven**, **chemical suppression** and a **peristaltic pump** for suppressor regeneration. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven/ChS/PP/Deg (2.930.2360)

The 930 Compact IC Flex Oven/ChS/PP/Deg is the intelligent Compact IC instrument with **column oven**, **chemical suppression** and a **peristaltic pump** for suppressor regeneration and built-in **degasser**. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven/SeS (2.930.2400)

The 930 Compact IC Flex Oven/SeS is the intelligent Compact IC instrument with **column oven** and **sequential suppression**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven/SeS/Deg (2.930.2460)

The 930 Compact IC Flex Oven/SeS/Deg is the intelligent Compact IC instrument with **column oven**, **sequential suppression** and built-in **degasser**. An 800 Dosino can be used for the regeneration of the suppressor. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven/SeS/PP (2.930.2500)

The 930 Compact IC Flex Oven/SeS/PP is the intelligent Compact IC instrument with **column oven**, **sequential suppression** and **peristaltic pump** for suppressor regeneration. The instrument can be used with any separation and detection methods.



930 Compact IC Flex Oven/SeS/PP/Deg (2.930.2560)

The 930 Compact IC Flex Oven/SeS/PP/Deg is the intelligent Compact IC instrument with **column oven**, **sequential suppression**, a **peristaltic pump** for suppressor regeneration and built-in **degasser**. The instrument can be used with any separation and detection methods.



Basic IC plus – Instruments

883 Basic IC plus (2.883.0020)

The 883 Basic IC plus is an intelligent, very compact ion chromatograph for education and routine analysis. For determining cations and anions with and without chemical suppression. Conductivity Detector, MagIC Net Basic software and textbook included.

883 Basic IC plus Package (2.883.1020)

Package for automated analysis with the 883 Basic IC plus. For education and routine analysis. For determining cations and anions with and without chemical suppression. 883 Basic IC plus, 863 Compact IC Autosampler, MagIC Net Basic software and textbook included.



Additional IC Vario components

Alternative IC components – Introduction

Ion chromatography has established itself in laboratories as a high-performance and flexible method. The range of analytes that can be determined is improved with additional IC components, and sensitivity and selectivity can be improved as well.

Heatable modules can be used not only for Metrohm Inline Sample Preparation (MISP) but also for post-column reaction systems. Data converters enable the import of external detector signals. On the other hand, analog signals can be output to external evaluation systems with the 891 Professional Analog Out.



Heatable reactors and column compartments

943 Professional Reactor Vario (2.943.0110)

The 943 Professional Reactor Vario is a heatable reactor, especially developed for pre- and post-column derivatization. It captivates by its robustness, the fast heating rate and the possibility of carrying out reactions at up to 150 °C.



943 Professional Thermostat Vario (2.943.0210)

The 943 Professional Thermostat Vario is a stand-alone column oven for up to two columns with a maximum length of 150 mm. It captivates by its fast heating rate and the possibility of operating two separation columns together at up to 80 °C.

Data Converters

771 IC Compact Interface (2.771.0010)

The universally applicable analog-digital converter with two channels and 24 Bit resolution. The data is passed along to the PC through the RS-232C interface and can be processed further there with IC Net or with MagIC Net.



771 IC Compact Interface; MagIC Net Professional (2.771.0110)

IC Compact Interface with the MagIC Net Professional software. The 771 Compact Interface combines the analog signal of the existing IC instruments (Compact, Modular, Advanced) with the improved possibilities of the modern MagIC Net software.



771 IC Compact Interface; MagIC Net Compact (2.771.0210)

IC Compact Interface with the MagIC Net Compact software. The 771 Compact Interface combines the analog signal of the existing IC instruments (Compact, Modular, Advanced) with the improved possibilities of the modern MagIC Net software.



891 Professional Analog Out (2.891.0010)

The 891 Professional Analog Out is an additional module for intelligent IC instruments. It allows to transfer analog signals of different chromatographic data to external data systems.



Professional IC Vario – Hyphenated systems

IC Vario coupling techniques – Introduction

The world of ion chromatography is extended considerably when Metrohm IC is coupled with other analysis methods, sample preparation techniques or detection systems.

The possibilities are practically unlimited. Any system that can process or supply aqueous solutions as samples can be coupled to Metrohm IC instruments.

This means that ion chromatography can be combined with Metrohm titrators and measuring instruments to form hyphenated systems. These TitrIC Vario or VoltIC Vario systems enable, for example, the entire water analysis, down to ion balance, simultaneously from a single sample. Additional typical examples include the coupling of the IC with MS or ICP-MS, the Combustion IC and air monitoring systems.



Hyphenated IC systems

TitriC Vario pro I – The basic hyphenated system for IC and titration (TitriC Vario pro I)

Fully automatic system for direct measurement of temperature, conductivity and pH value; the titrimetric determination of p value, m value, calcium and magnesium and the determination of anions by ion chromatography.



TitriC Vario pro II – The hyphenated IC and titration system for comprehensive anion and cation analysis (TitriC Vario pro II)

Fully automatic system for direct measurement of temperature, conductivity and pH value; the titrimetric determination of p and m value, the determination of cations including calcium and magnesium, as well as anions by ion chromatography.



TitriC Vario pro III – The professional hyphenated IC and titration system with lockable sample vessels (TitriC Vario pro III)

Fully automatic system for direct measurement of temperature, conductivity and pH value; the titrimetric determination of p and m value, the determination of cations including calcium and magnesium, as well as anions by ion chromatography. The sample changer is equipped with the DisCover function for automatic sample vessel cover removal.



VoltIC Vario pro I – The hyphenated IC and voltammetry system for parallel determination of anions, cations and heavy metals (VoltIC Vario pro I)

VoltIC Vario I is the perfect combination of IC and voltammetry for simultaneous determination of anions, cations and heavy metals. MagIC Net controls IC instruments, starts voltammetric determination, and summarizes the results from IC and voltammetry.



930 Metrohm Combustion IC (2.930.9010)

The 930 Metrohm Combustion IC enables the analysis of halogens and sulfur in flammable samples of all types using inline combustion digestion with subsequent ion chromatography determination (Combustion IC). It includes all required components. If necessary, the 930 Metrohm Combustion IC package can be supplemented with an Autosampler for solid or liquid samples (MMS 5000 Autosampler). The entire analysis, including sample input and combustion, is completely controlled by MagIC Net.




920 Absorber Module (2.920.0010)

The 920 Absorber Module combines the Combustion Module with the ion chromatograph. The 920 Absorber Module ensures that the gaseous compounds of the analytes are dissolved and channeled to the IC. It is responsible for the entire Liquid Handling. In addition to Combustion IC, it can also be used for gas analysis.



MMS 5000 Autosampler (2.136.0800)

MMS 5000 Autosampler from Analytik Jena for use with the Metrohm Combustion IC for fully automatic analysis of liquid and solid samples. In order to match the modular Multi-Matrix sampler with the correct sample type, either the liquid kit (6.7303.000) or the solid kit (6.7302.000) must be used.

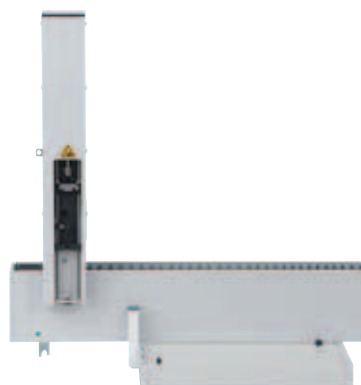

Combustion Module (Oven + ABD) (2.136.0700)

The Combustion Module (Oven + ABD) enables the sample digestion of flammable samples of all types under pyrolysis and oxidation. The Combustion Module is comprised of the combustion oven and the Auto Boat Driver (automatic sample introduction). Both are products of Analytik Jena which have been optimized specially for coupling with ion chromatographs.



Auto Boat Drive (2.136.0710)

The Auto Boat Drive (ABD) automatically guides the sample scoops into the combustion oven. The sample injection into the boat can proceed manually or with a corresponding sampler. The Analytik Jena product has been optimized specially for coupling with ion chromatographs.



LPG/GSS Module (2.136.0720)

The LPG/GSS Module is a sample injection system for either liquefied gases or gases under enhanced pressure. The module is controlled automatically and moves the respective amounts of gas to the combustion oven for combustion. The Analytik Jena product has been optimized specially for coupling with ion chromatographs.



Combustion Module (Oven + LPG/GSS) (2.136.0730)

The Combustion Module (Oven + LPG/GSS) enables sample digestion during the pyrolysis of liquefied gases and gases under pressure. The Combustion Module (Oven + LPG/GSS) is comprised of the combustion oven and the LPG/GSS module. Both are products of Analytik Jena which have been optimized specially for coupling with ion chromatographs.



PILS, Particle Into Liquid Sampler (2.136.0400)

Coupling with ion chromatographs allows automatic determination of the ionic composition of the aerosols without requiring additional sample preparation.



MARGA, Monitor for AeRosols and Gases in ambient Air (MARGA)

MARGA is a fully automated online system that determines anions and cations in gases and aerosols. The acid and alkali gases are absorbed in water in a „Wet Rotating Denuder“ and the aerosols in a „Steam Jet Aerosol Collector“ and investigated with two Compact ICs for their anion and cation content. MARGA is designed for prolonged autonomous operation.

MARGA is distributed by Applikon (www.metrohm-applikon.com).



Automation in ion chromatography

Overview of IC automation

Sample changers

Automation in ion chromatography ranges all the way from simple automatic sample injection to complex sample preparation with combined methods. It must be possible to process sample quantities ranging from a few μL to several mL. A number of sample changers with different areas of application are available for this purpose.

The 858 Professional Sample Processor is more than just a sample changer. Equipped with pumps, high-pressure valve and Dosinos, it makes an integral contribution to Inline Sample Preparation and Liquid Handling.

In addition to the 858 Professional Sample Processor, the 889 IC Sample Center, the 919 IC Autosampler plus, the 863 Compact IC and the entire series of the 814 and 815 Sample Processors are available from the titration range.

Metrohm Inline Sample Preparation (MISP)

Samples such as milk, chocolate, caustic soda, biodiesel or heavily contaminated waste waters require sample preparation before they can be analyzed with IC. Together with the 858 Professional Sample Processor, the 940 Professional IC Vario offers extensive possibilities for completely automated Inline Sample Preparation, e.g., Inline Ultrafiltration, Inline Dialysis, Inline Preconcentration, Inline Matrix Elimination, Inline Matrix Neutralization and Inline Calibration.



IC Automation – Instruments

858 Professional Sample Processor (2.858.0010)

The 858 Professional Sample Processor processes samples from 500 μL to 500 mL. The sample transfer takes place either by means of a peristaltic pump on the 850 Professional IC system or with an 800 Dosino.



858 Professional Sample Processor – Pump (2.858.0020)

The 858 Professional Sample Processor – Pump processes samples from 500 μL to 500 mL. The sample transfer takes place either with the installed bidirectional two-channel peristaltic pump or with an 800 Dosino.



858 Professional Sample Processor – Pump – Injector (2.858.0030)

The 858 Professional Sample Processor – Pump – Injector processes samples from 500 μL to 500 mL. The sample transfer takes place either with the installed bidirectional two-channel peristaltic pump or by means of an 800 Dosino. In addition, a six-way injection valve is available for the sample preparation.



919 IC Autosampler plus (2.919.0020)

The 919 IC Autosampler plus fulfills the requirements of laboratories with medium sample numbers. It enables automation of the full range of Metrohm IC instruments.




863 Compact IC Autosampler (2.863.0010)

The 863 Compact IC Autosampler is the ideal help for routine analysis. It enables automation of the full range of Metrohm IC instruments.



815 Robotic Soliprep for LC (2.815.4110)

The 815 Robotic Soliprep for LC is a complete system for the completely automatic preparation of samples which need to be dissolved, homogenized, diluted or filtered prior to their determination. The samples are conveyed directly into the injector of the chromatograph after preparation.

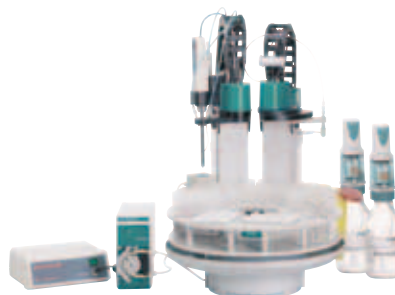

889 IC Sample Center (2.889.0010)

The 889 IC Sample Center is a robust Autosampler for high sample throughput, optimized for the challenges of the modern analytic laboratory. It works in accordance with the x-y-z principle and a syringe control with high resolution for precise sample injection. A double needle system enables the penetration of vessel caps and septa. A PEEK injection valve completes the automation system of the 889 IC Sample Center. It is the appropriate automation solution when you have only a very small amount of sample.



889 IC Sample Center – cool (2.889.0020)

The 889 IC Sample Center – cool is the appropriate automation solution when you have only a very small amount of sample. In comparison with the 889 IC Sample Center, it possesses in addition a cooling function and is thus the ideal sample changer for biochemically relevant or thermally unstable samples.



Additional Sample Processors for IC

Even more flexibility and choice!

Even the USB Sample Processors of the titration segment can be actuated with **Magic Net**. This means that there are practically no limits to automation in ion chromatography. Whether it be small or large sample vessels, whether it be at room temperature or cooled, whether it be automatic sample preparation with one or two sample changer towers – the answer in ion chromatography is always:

Yes, we can do it!

The advantages of a sample changer lie not only in the time savings for the laboratory personnel: Automatic systems control operating sequences and thus improve **reproducibility and accuracy**. Errors can be reduced to a minimum.

The system works through the prepared samples, no matter what time of day it is. Whether it be automatic sample preparation, Liquid Handling or sample processing – this Sample Processor generation controls everything that one previously associated only with laboratory robots.

Depending on preference, the USB Sample Processor can be controlled not only with **Magic Net** but also with **Touch Control**, **PC Control** or conveniently with the **tiamo™** titration software.



814 USB Sample Processor with sample rack for 12 x 250 mL

Ordering Information

2.814.0010	814 USB Sample Processor (1T/1P)
2.814.0020	814 USB Sample Processor (1T/2P)
2.814.0030	814 USB Sample Processor (1T/0P)
2.814.0110	814 USB Sample Processor (2T/2P)
2.814.0120	814 USB Sample Processor (2T/4P)
2.814.0130	814 USB Sample Processor (2T/0P)
2.815.0010	815 Robotic USB Sample Processor XL (1T/1P)
2.815.0020	815 Robotic USB Sample Processor XL (1T/2P)
2.815.0030	815 Robotic USB Sample Processor XL (1T/0P)
2.815.0110	815 Robotic USB Sample Processor XL (2T/2P)
2.815.0120	815 Robotic USB Sample Processor XL (2T/4P)
2.815.0130	815 Robotic USB Sample Processor XL (2T/0P)
2.815.2110	815 Robotic Flexible Soliprep
2.815.3110	815 Robotic Filtration Soliprep

Liquid Handling in ion chromatography

Liquid Handling in IC – Introduction

Sample input – Inline Sample Preparation

In the beginning was the *syringe* – manual sample injection continues to be used today. In most cases, however, the samples are transferred automatically into the ion chromatograph. It begins with the simple *peristaltic pump* that pumps the sample solution to the injector. Additional components, e.g., valves, filtration and dialysis cells, neutralization modules, etc. thus pave the way to Inline Sample Preparation. The use of the **800 Dosino** as module for sample transfer, also and in particular for the exact dosing of several solutions and different volumes, represents yet another massive extension of these possibilities. Logical and flexible dilution – that means free selection of dilution factor and repeated dilution of the sample when the result lies outside of the calibration range – high-precision „Partial-Loop Injection“ methods and automatic calibration with variable preconcentration – enables a calibrated working range of up to six decades (e.g., 10 ppt to 10 ppm); these are only a few of the many applications that only became possible with the advent of the 800 Dosino.

IC equipment for Liquid Handling

MISP made simple. The IC equipments contain all of the parts required for the respective sample preparation method. This way you can be sure that the method also works.

Liquid Handling for IC

800 Dosino (2.800.0010)

Drive with write/read hardware for intelligent Dosing Units. With fixed cable (length 150 cm).



846 Dosing Interface (2.846.0010)

USB-capable control unit for connecting a maximum of four 800 Dosinos or 805 Dosimats for dosing and Liquid Handling tasks. A Touch Control or the connection to a PC with *tiamo*[™], MagIC Net, viva or 797 VA Computrace is required for operation.



IC equipment: Additional eluent on the Eluent Production Module (6.5330.090)

Accessory set for Eluent Production Module. Contains all parts necessary for expansion by one eluent. The level sensor must be ordered in accordance with the application.




IC equipment: Inline dialysis (6.5330.100)

Accessory set for Inline Dialysis. For use with the 858 Professional Sample Processor and an additional 2-channel peristaltic pump.



IC equipment: Inline ultrafiltration (6.5330.110)

Accessory set for Inline Ultrafiltration. For use with the 858 Professional Sample Processor.

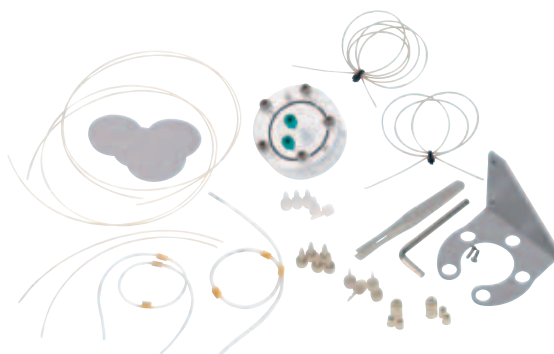

IC equipment: Inline dilution (6.5330.120)

Accessory set for Inline Dilution. For use with the 858 Professional Sample Processor, 800 Dosino and 741 Magnetic Stirrer.



IC equipment: Liquid Handling Station, left (6.5330.130)

Accessory set for assembling the Liquid Handling Station on the Professional Sample Processor. The rinsing water supply can be accomplished by means of a peristaltic pump or a Dosino.



IC equipment: MiPCT (6.5330.140)

Accessory set for Inline Preconcentration (MiPCT) including Liquid Handling Station, left.



IC equipment: Dose-in Gradient (6.5330.150)

Accessory set for assembling the Dose-in Gradient.



IC equipment: MiPCT-ME (6.5330.160)

Accessory set for assembling a Dosino for Metrohm intelligent Preconcentration Technique with Matrix Elimination (MiPCT-ME).



IC equipment: MiPUT (6.5330.170)

Accessory set for assembling a Dosino for Sample Pickup.




IC equipment: MiPT (6.5330.180)

Accessory set for assembling a Dosino for Partial-Loop-Injection.



IC equipment: Dosino regeneration (6.5330.190)

Accessory set for the assembly of a Dosino for automatic regeneration of the Metrohm Suppressor Module (MSM).

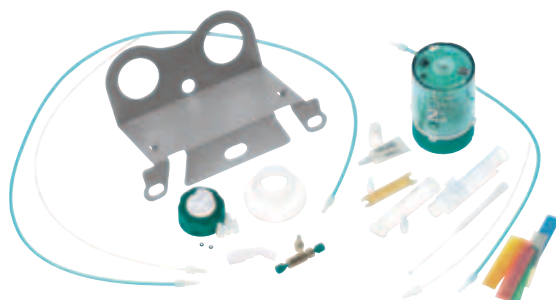

IQ/OQ Kit for IC (6.5333.000)

The IQ/OQ Kit contains all parts and standard solutions required for IQ/OQ in ion chromatography.




IC equipment for Liquid Handling Set for PILS
(6.5335.000)

Accessories set for PILS (Particle Into Liquid Sampler).



Peristaltic pump, 8-channel (2.136.0500)

8-channel peristaltic pump for PILS (Particle Into Liquid sampler) for transferring any auxiliary solution.

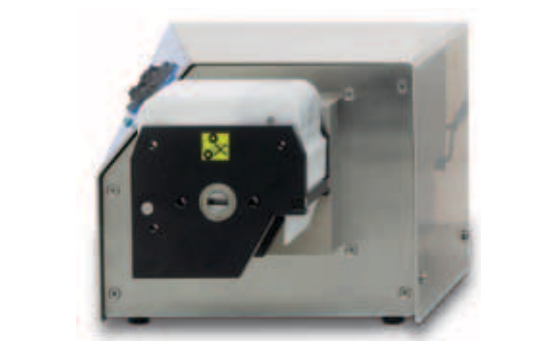

Professional Vario IC – Software

MagIC Net – Introduction

MagIC Net software for intuitive and simple operation

It's MagIC!

Clear symbols, clear presentation, intuitive operation, „One-Button IC“: This is MagIC Net.

Complete system monitoring, control charts for measurements, convenient database functions: This, too, is MagIC Net, the intelligent software – Swiss Made – for controlling and monitoring the Metrohm ion chromatography systems.

The MagIC Net chromatography software controls all intelligent ion chromatographs and records all the data that arises. The current version of MagIC Net is offered in four different versions:

- MagIC Net Professional supports the entire range of intelligent ion chromatographs and sample changers. This means that all of the peripheral devices for Inline Sample Preparation and Liquid Handling can also be operated and other Metrohm instruments or third-party devices that are already in use can be remote-controlled.
- MagIC Net Compact comprises the complete functionality of the MagIC Net Professional version. However, only the Compact IC instruments and one sample changer can be connected for automation purposes.
- MagIC Net Multi makes MagIC Net Professional available in its entirety as a client-server installation.
- MagIC Net Basic is a special version for the 883 Basic IC plus, modified for training requirements. MagIC Net Basic is contained in the instrument.

All four versions are exceptional for their clearly organized presentation, clear symbols and intuitive operation. The checking and monitoring functions of the MagIC Net software are unique: All system parameters, service intervals or expiration data can be checked, as can also all measuring results of samples and standard solutions. When a limit value is exceeded, previously defined actions, e.g., the sending of a message via e-mail or cellular phone or the switching off of the system, can be triggered. Thanks to the modern data management of MagIC Net, one never loses sight of the larger picture, as

all of the information required is made available immediately.

All intelligent components are recognized, monitored and actuated automatically:

- IC Amperometric Detector
- IC Conductivity Detector
- iCell
- iColumns
- iReactor
- 771 Compact Interface
- 800 Dosinos
- 814/815 Robotic USB Sample Processors
- 846 Dosing Interface
- 850 Professional IC
- 858 Professional Sample Processor
- 863 Compact IC Autosampler
- 872 Extension Module
- 881 Compact IC pro
- 882 Compact IC plus
- 883 Basic IC plus
- 886 Professional Reactor / Thermostat
- 887 Professional UV/VIS Detector
- 889 IC Sample Center
- 891 Professional Analog Out
- 896 Professional Detector
- 919 IC Autosampler plus
- 930 Compact IC Flex
- 940 Professional IC Vario
- 941 Eluent Production Module
- 942 Extension Module Vario
- 943 Professional Reactor/Thermostat Vario
- 944 Professional UV/VIS Detector Vario
- 945 Professional Detector Vario

Flexible programming of the sequences in the time programs, combined with logical decisions and virtually infinite calculation possibilities, open up the entire world of ion chromatography with MagIC Net. From simple routine applications all the way to highly complex combinations of different sample preparation techniques.

MagIC Net versions

MagIC Net 3.0 Compact CD: 1 license (6.6059.301)

Professional PC program for controlling an intelligent Compact IC instrument, one detector and one Autosampler, or a 771 Compact Interface. The software permits control, data acquisition, data evaluation and data monitoring as well as report generation of ion chromatographic analyses. MagIC Net Compact complies fully with FDA Regulation 21 CFR Part 11 as well as GLP. MagIC Net is available in 14 dialog languages.



MagIC Net 3.0 Professional CD: 1 license (6.6059.302)

Professional PC program for controlling all of the intelligent Professional IC systems, Compact IC instruments and their peripherals, such as various Autosamplers, 800 Dosino, 771 Compact Interface, etc. The software permits the control, data acquisition, data evaluation, data monitoring and report generation of ion chromatographic analyses. MagIC Net Professional complies fully with FDA Regulation 21 CFR Part 11 as well as GLP. MagIC Net is available in 14 dialog languages.



MagIC Net 3.0 Multi CD: 3 licenses (6.6059.303)

Professional PC program for controlling all of the intelligent Professional IC systems, Compact IC instruments and their peripherals, such as various Autosamplers, 800 Dosino, 771 Compact Interface, etc. The software permits the control, data acquisition, data evaluation, data monitoring and report generation of ion chromatographic analyses. MagIC Net Multi complies fully with FDA Regulation 21 CFR Part 11 as well as GLP. MagIC Net is available in 14 dialog languages. Client/server version with 3 licenses.



Metrohm IC Driver for Empower (6.6070.000)

Software driver for integrating Metrohm IC instruments in „Empower“ from Waters.





Metrohm Quality Service

Metrohm Quality Service

Reliable measurement results for the lifetime of the instrument

It makes no difference whatsoever whether you perform water analysis with the 940 Professional IC Vario or trace analysis with VA or whether you determine water contents in your pharmaceuticals laboratory with Karl Fischer titration, our Metrohm Quality Service ensures that you can rely 100% on your measurement results for the entire lifetime of the instrument.

Preventive maintenance – just as important as with your car

Preventive maintenance carried out on a regular basis extends your analysis systems' trouble-free lifetime and operational capability. Qualification training-certified service technicians perform the maintenance work worldwide. You can select between different types of service contracts. A full service contract, for example, offers you maximum security for troublefree work, while giving you complete control of costs and providing fully compliant documentation.

Metrohm Compliance Service

The variety of different laboratory instruments and analysis systems in use today makes compliance with statutory requirements very complicated for companies operating in the regulated sector. Put your trust therefore in the Metrohm Compliance Service when the time comes for the professional initial qualification of your analyzers. As an experienced and trustworthy partner, Metrohm provides your customers rapidly and professionally with everything required for compliance with regulations. Our qualification and validation documents and our services provide you with support for compliance with the requirements of FDA regulations, GLP/GMP standards and GAMP directives.





Metrohm Quality Service

With Metrohm Quality Service you are on the safe side from day one. From installation to start-up, to regular maintenance and – if problems arise – to quick repair, we guarantee you precise and correct measuring results.

Metrohm Quality Service	Customer benefits
Metrohm Care Contracts	<ul style="list-style-type: none"> • Minimizes downtime through preventative maintenance • Cost control and savings through free or discounted replacement materials and consumables • Guaranteed reaction times and rapid on-site repair • Documented instrument certification as an ideal preparation for audits
Metrohm Software Maintenance	<ul style="list-style-type: none"> • High data security and maximum system performance through regular, professional software maintenance
Metrohm Compliance Service	<ul style="list-style-type: none"> • Customized services and documentation for analytical instrument qualification (AIQ) • Professional start-up (IQ/OQ or Certified Installation) and requalification or recertification by specifically trained employees
Metrohm Remote Support	<ul style="list-style-type: none"> • Quick resolution of software and application issues directly at the workplace
Metrohm Dosing Test	<ul style="list-style-type: none"> • Calibration of burettes (e.g., dosing and exchange units) with certification • Accurate measurement results • Verification documentation for compliance with regulations and efficient audits
Metrohm Repair Service	<ul style="list-style-type: none"> • Rapid availability of repaired instruments thanks to decentralized repair workshops around the world and a central workshop at the manufacturer site • Highly qualified service technicians ensure sustainable repair success • Rapid resolution of problems and minimized downtimes through on-site emergency services and express repairs
Metrohm Spare Parts	<ul style="list-style-type: none"> • Original spare parts, made in Switzerland and available worldwide • Short delivery times through warehousing from local distributors • Investment security through ten-year spare parts guarantee after discontinuation
Metrohm Application Support	<ul style="list-style-type: none"> • Access to Metrohm Applications expertise (Application Bulletins, Application Notes, monographs, technical posters and specialized articles) • Rapid and professional resolution of any application issues through personal consultations with our specialists by e-mail, telephone, or remote support • Support for the solution of complex analytical problems, as well as method optimization on-site or at our application laboratory
Metrohm Training Programs	<ul style="list-style-type: none"> • Basic and advanced training with local representatives, at the Metrohm Academy or directly on-site • Efficient and proper use of all analytical methods, as well as results reliability through competently trained users • Training documentation and certificates for trouble-free audits

www.metrohm.com